
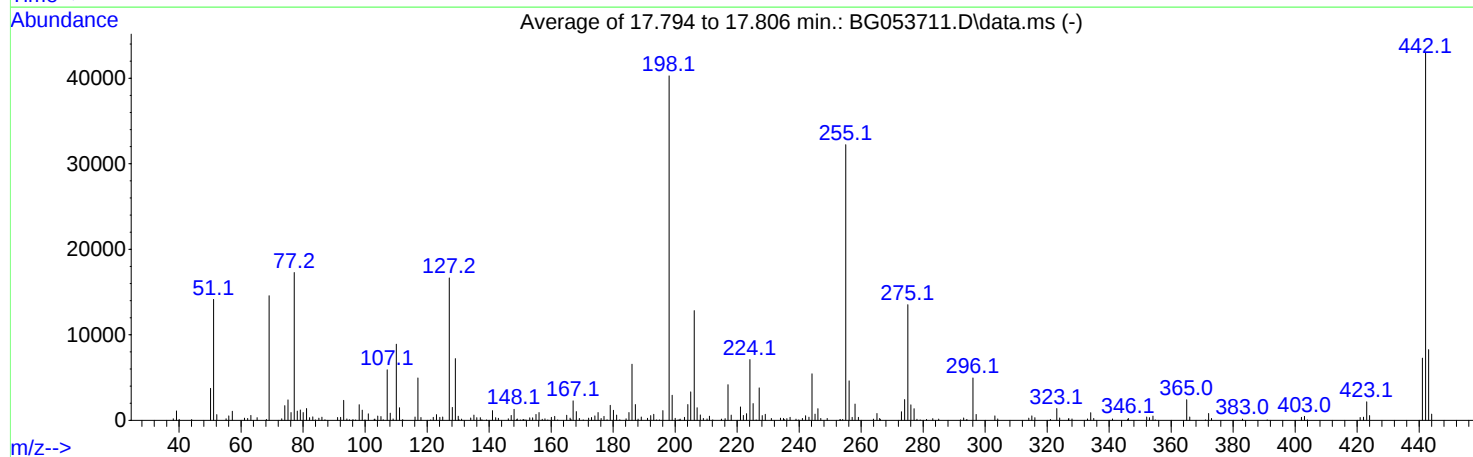


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052622\
 Data File : BG053711.D
 Acq On : 26 May 2022 10:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 15:11:41 2022

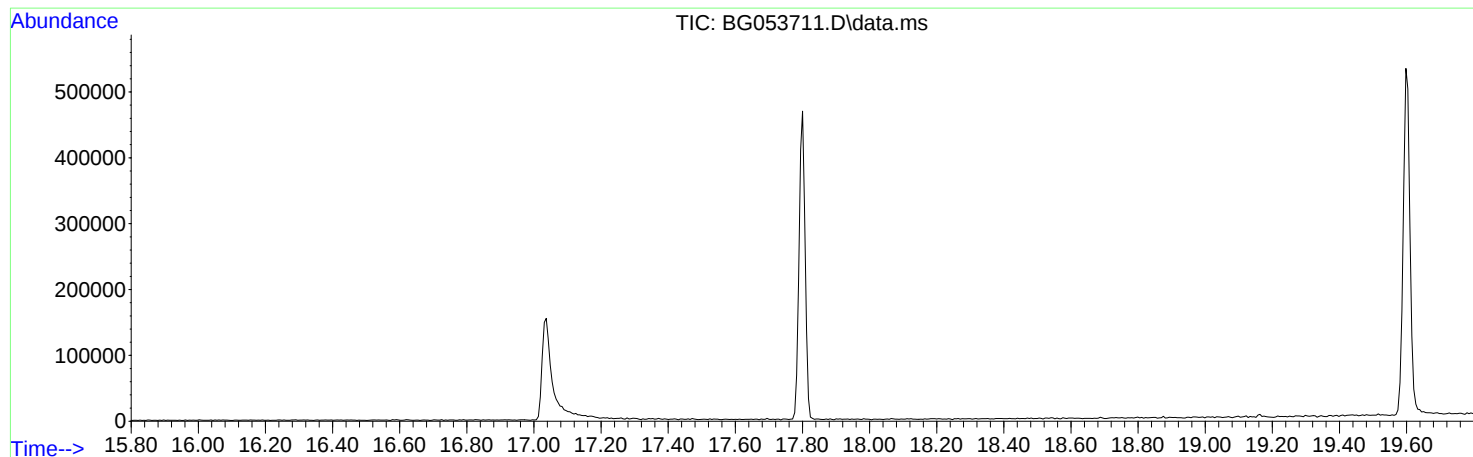




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	14141	PASS
68	69	0.00	2	0.7	107	PASS
69	198	0.00	100	36.2	14579	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.4	16659	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40272	PASS
199	198	5	9	7.3	2946	PASS
275	198	10	60	33.6	13533	PASS
365	198	1	100	6.0	2406	PASS
441	198	0.01	100	18.1	7283	PASS
442	442	50	100	100.0	43008	PASS
443	442	15	24	19.2	8262	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052622\
Data File : BG053711.D
Acq On : 26 May 2022 10:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 26 16:05:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

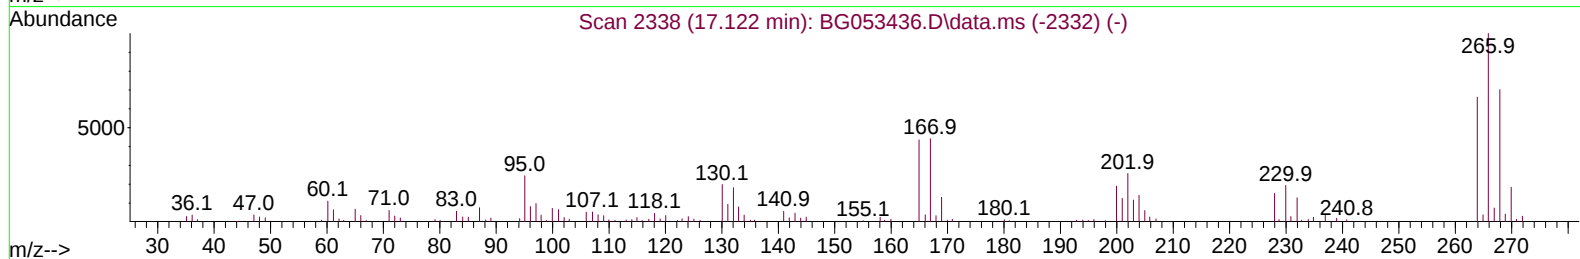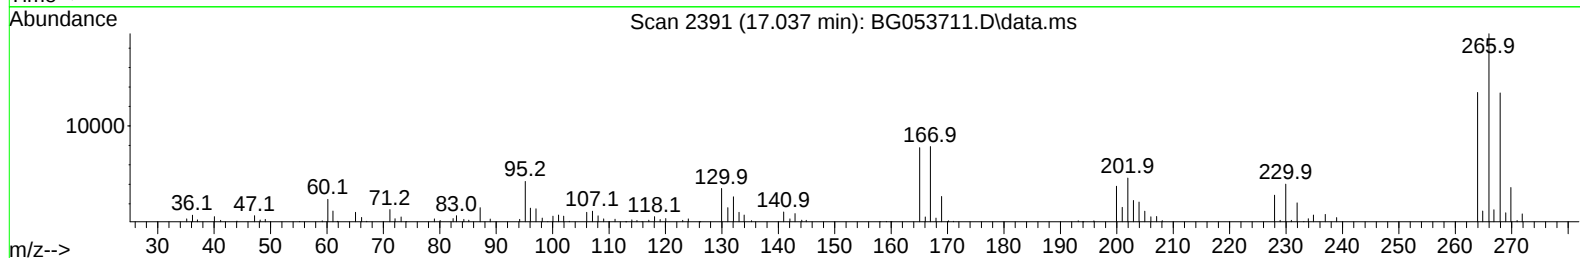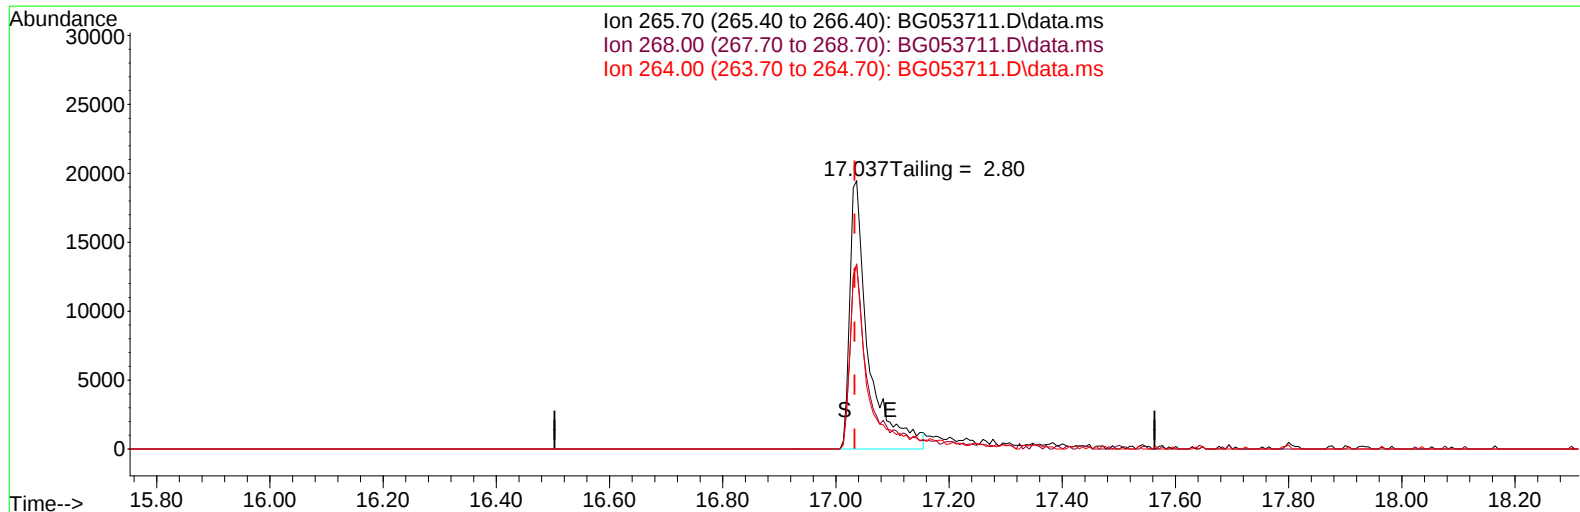

TIC: BG053711.D\data.ms

(70) Pentachlorophenol (C)

17.037min (+ 0.004) 98555.56 ng




response 46847

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	68.77
264.00	66.20	69.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052622\
Data File : BG053711.D
Acq On : 26 May 2022 10:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 26 16:05:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

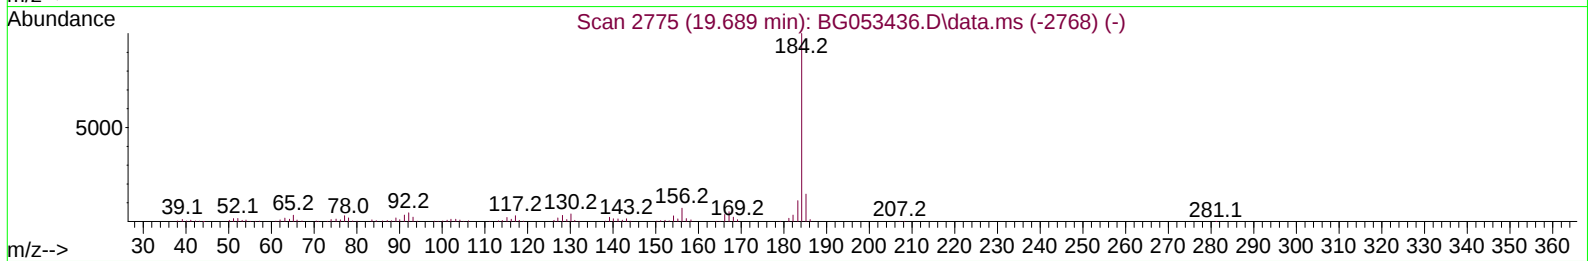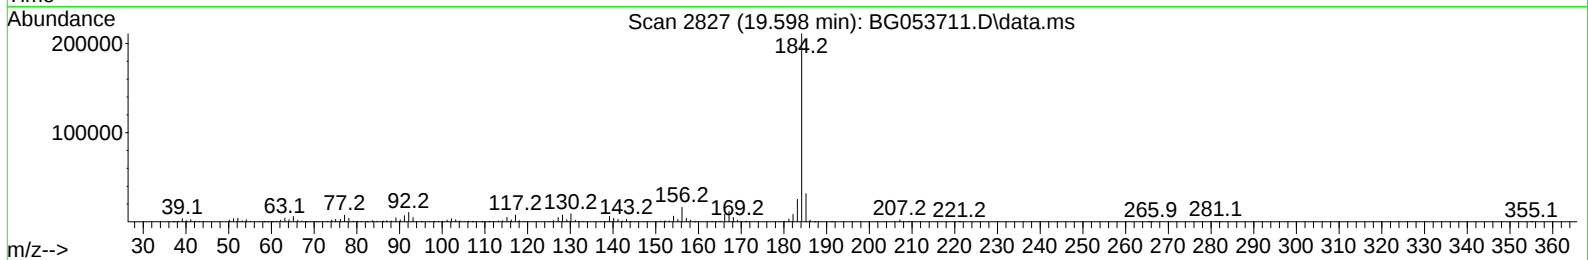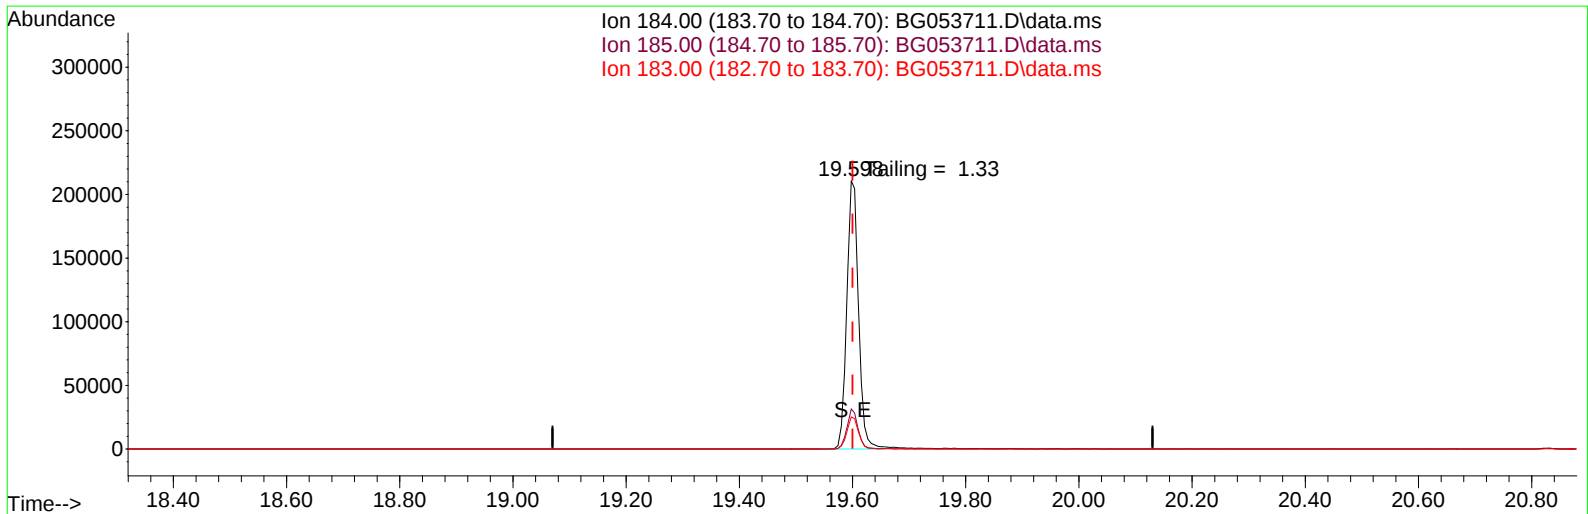

TIC: BG053711.D\data.ms

(77) Benzidine

19.598min (-0.002) 204321.53 ng

response 303868

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.01
183.00	11.10	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/26/2022	BNA_G	<u>BG053711.D</u>
Compound Name	Response	Retention Time
DDT	138903	20.82
DDD	576	20.39
DDE	68	19.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
644	139547	0.46

Instrument :
BNA_G
ClientSampleId :
DFTPP