
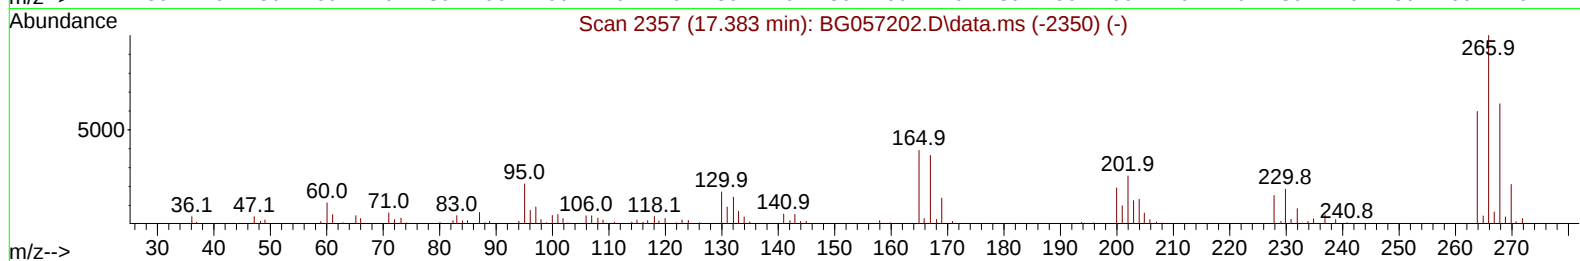
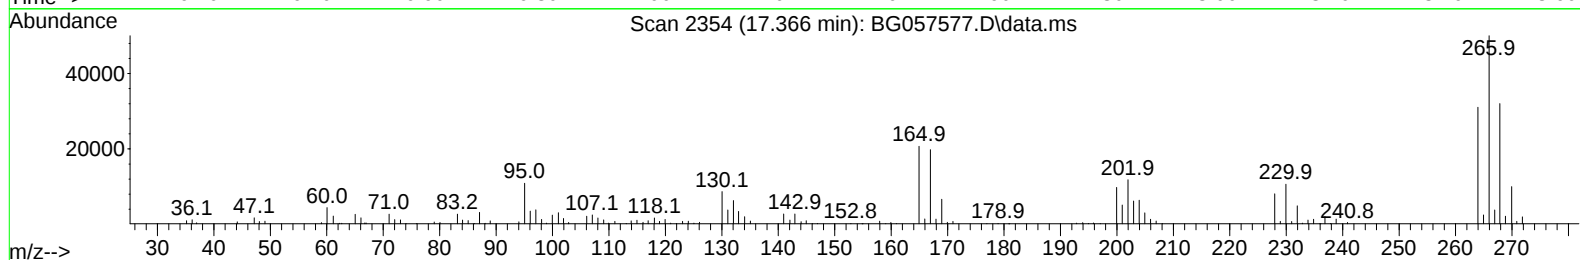


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052623\  
Data File : BG057577.D  
Acq On : 26 May 2023 9:08  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 11:07:08 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG042723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 26 02:58:05 2023  
Response via : Initial Calibration

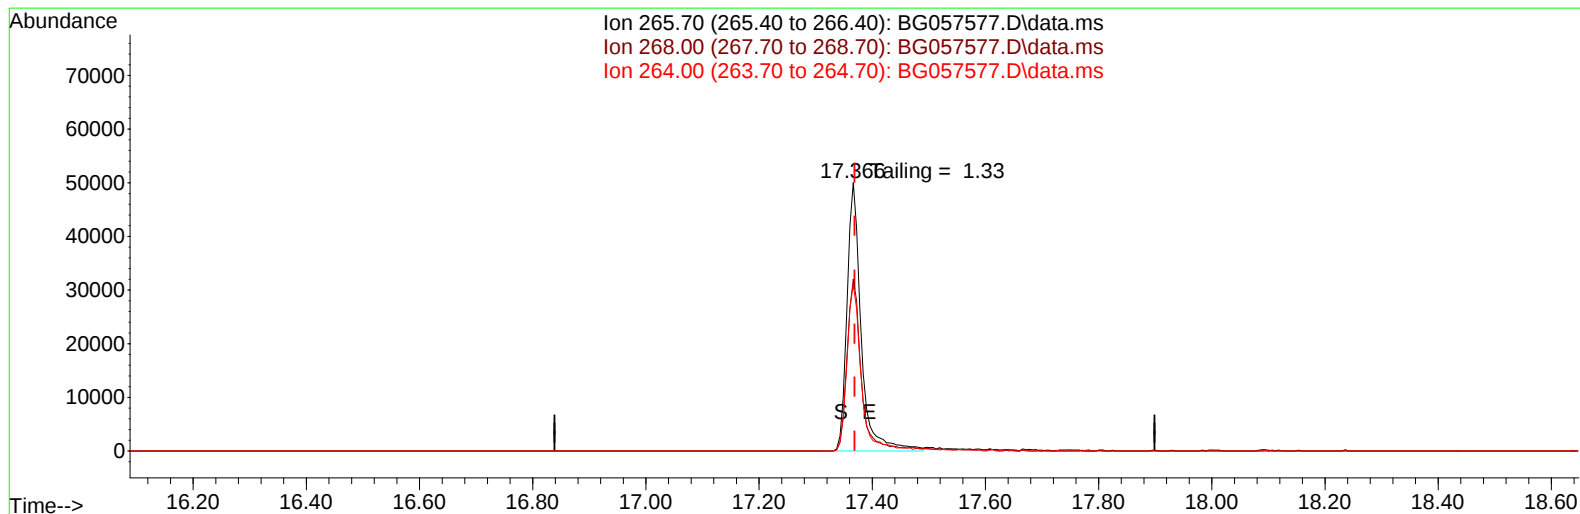

TIC: BG057577.D\data.ms

**(70) Pentachlorophenol (C)**




17.366min (-0.002) 32276.36 ng

response 87384

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 64.07  |
| 264.00 | 59.70  | 62.05  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052623\  
 Data File : BG057577.D  
 Acq On : 26 May 2023 9:08  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 11:07:08 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG042723.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri May 26 02:58:05 2023  
 Response via : Initial Calibration

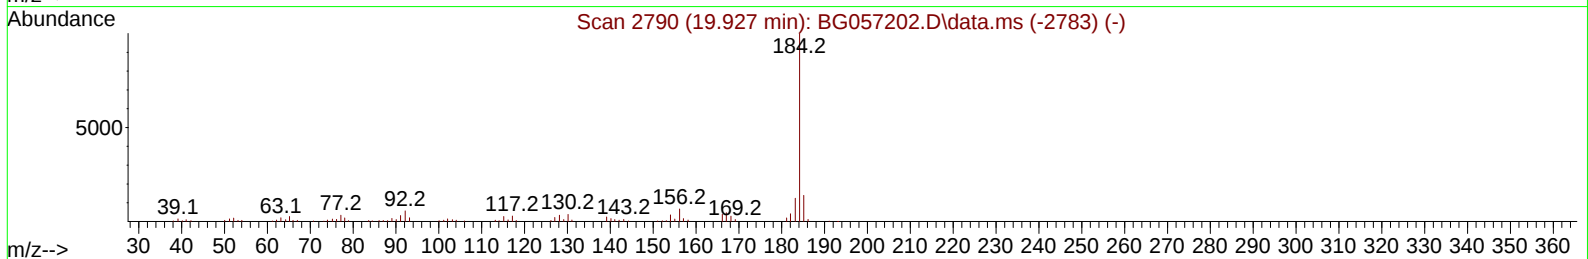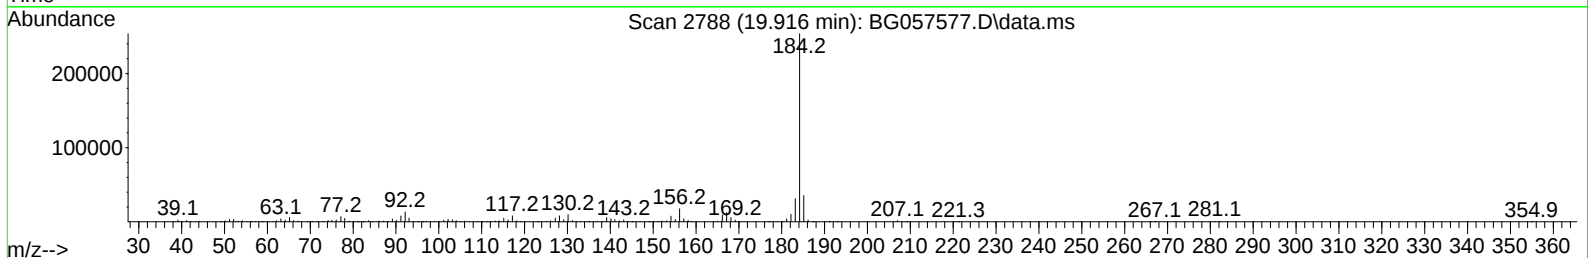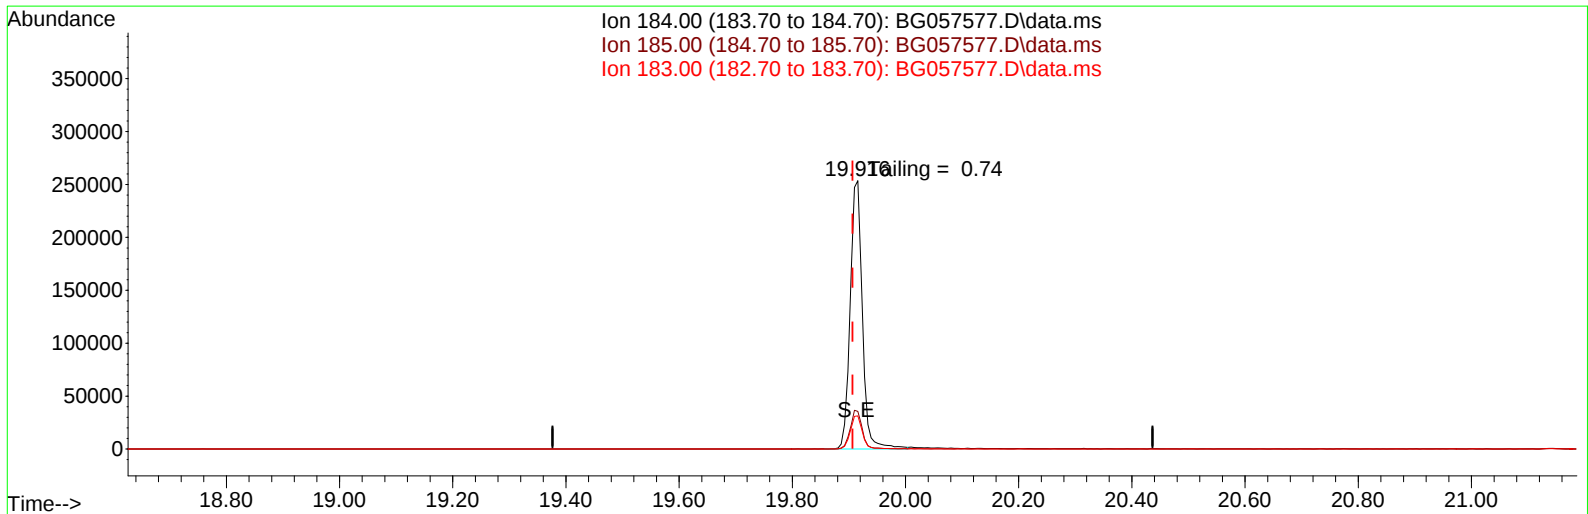

TIC: BG057577.D\data.ms

**(77) Benzidine****19.916min (+ 0.010) 0.00 ng****response 382715**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.90  | 14.04  |
| 183.00 | 12.40  | 12.35  |
| 0.00   | 0.00   | 0.00   |