
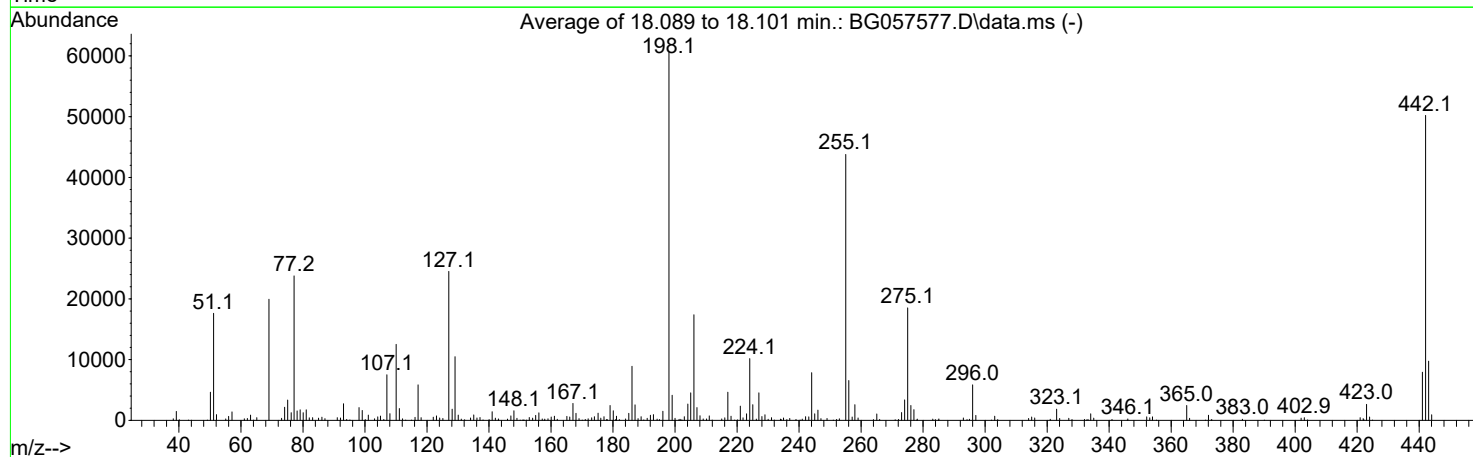


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052623\
Data File : BG057577.D
Acq On : 26 May 2023 9:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 26 02:58:05 2023

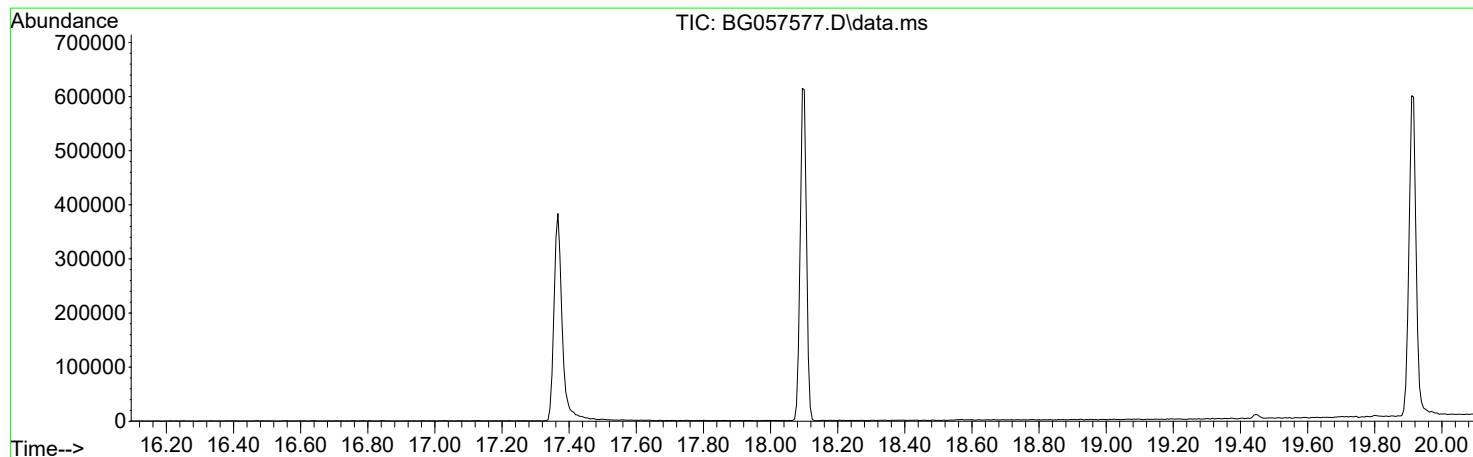

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	17622	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.9	19941	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.5	24525	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60563	PASS
199	198	5	9	6.8	4127	PASS
275	198	10	60	30.6	18531	PASS
365	198	1	100	4.0	2451	PASS
441	198	0.01	100	13.1	7939	PASS
442	442	50	100	100.0	50208	PASS
443	442	15	24	19.4	9750	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/26/2023	BNA_G	<u>BG057577.D</u>
Compound Name	Response	Retention Time
DDT	190827	21.144
DDD	7764	20.685
DDE	671	20.186
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8435	199262	4.23

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052623\
Data File : BG057577.D
Acq On : 26 May 2023 9:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 26 11:07:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 02:58:05 2023
Response via : Initial Calibration

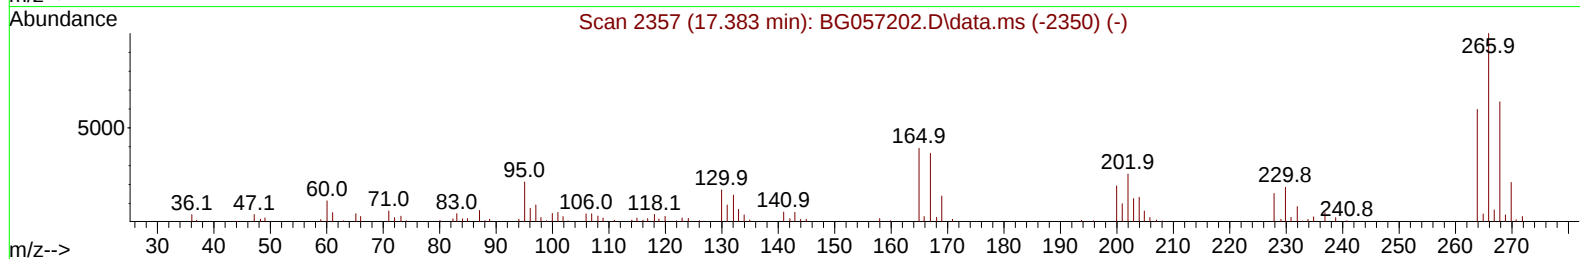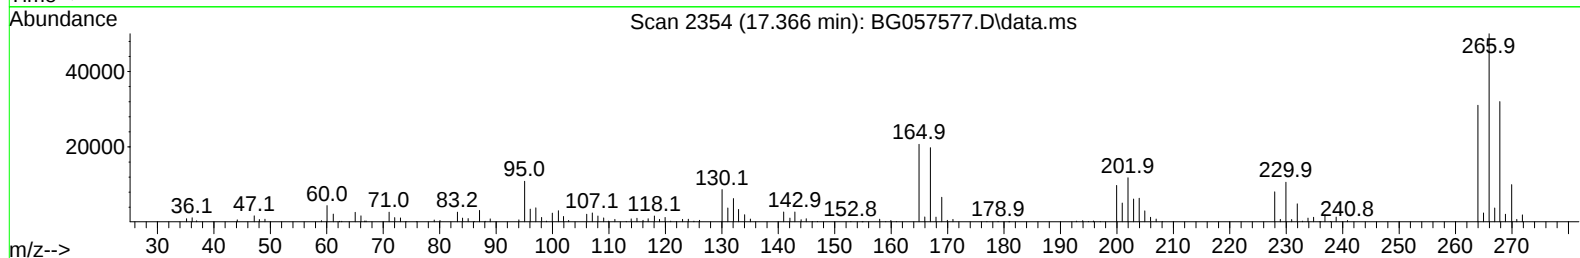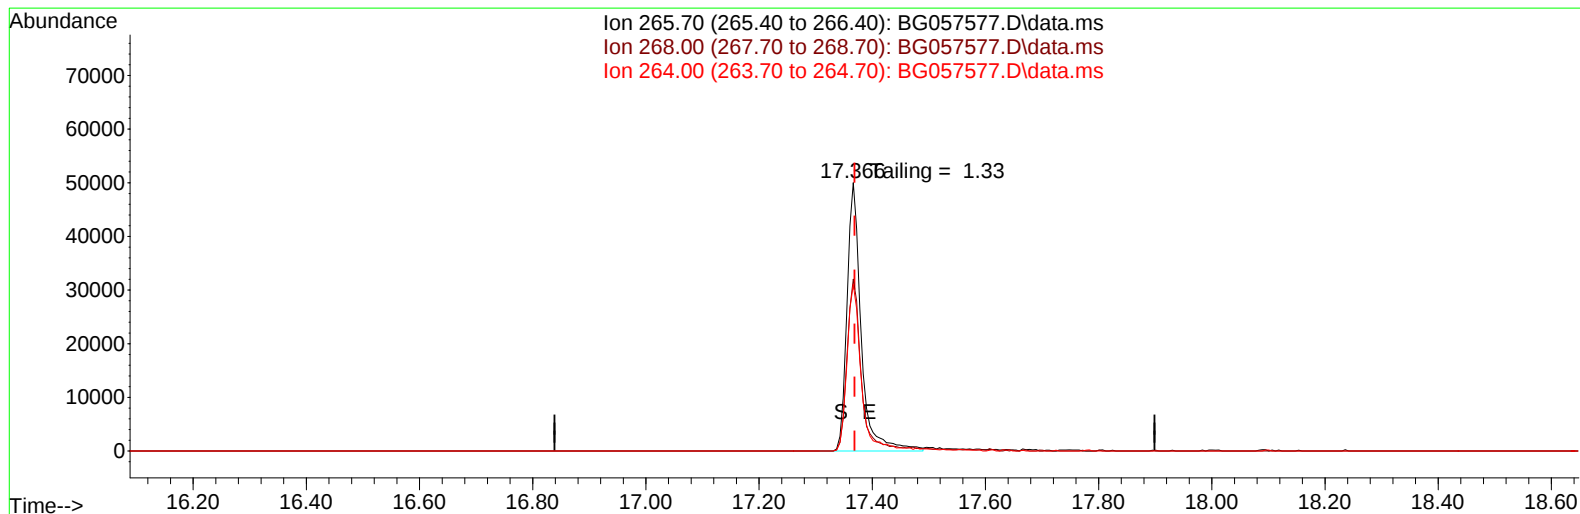

TIC: BG057577.D\data.ms

(70) Pentachlorophenol (C)

17.366min (-0.002) 32276.36 ng




response 87384

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.07
264.00	59.70	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052623\
Data File : BG057577.D
Acq On : 26 May 2023 9:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 26 11:07:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 02:58:05 2023
Response via : Initial Calibration

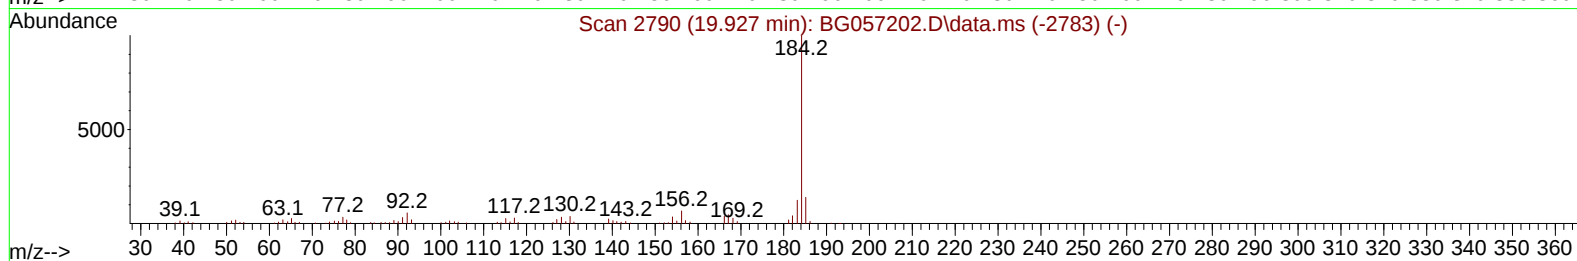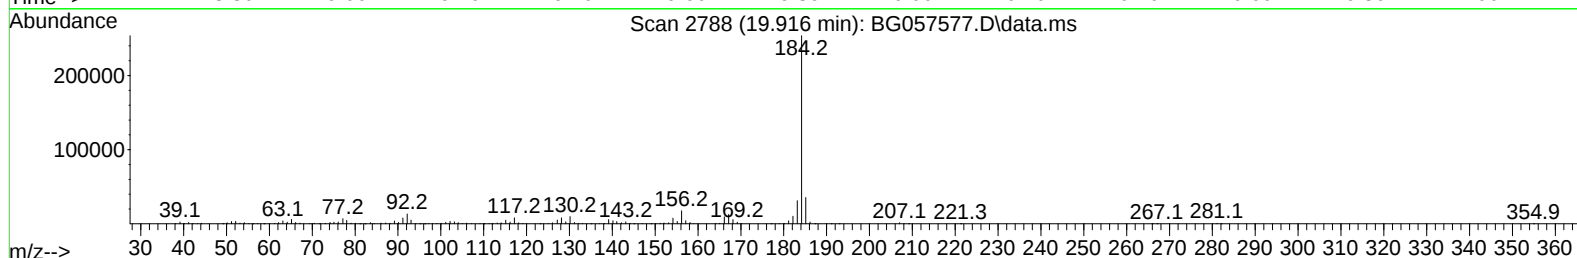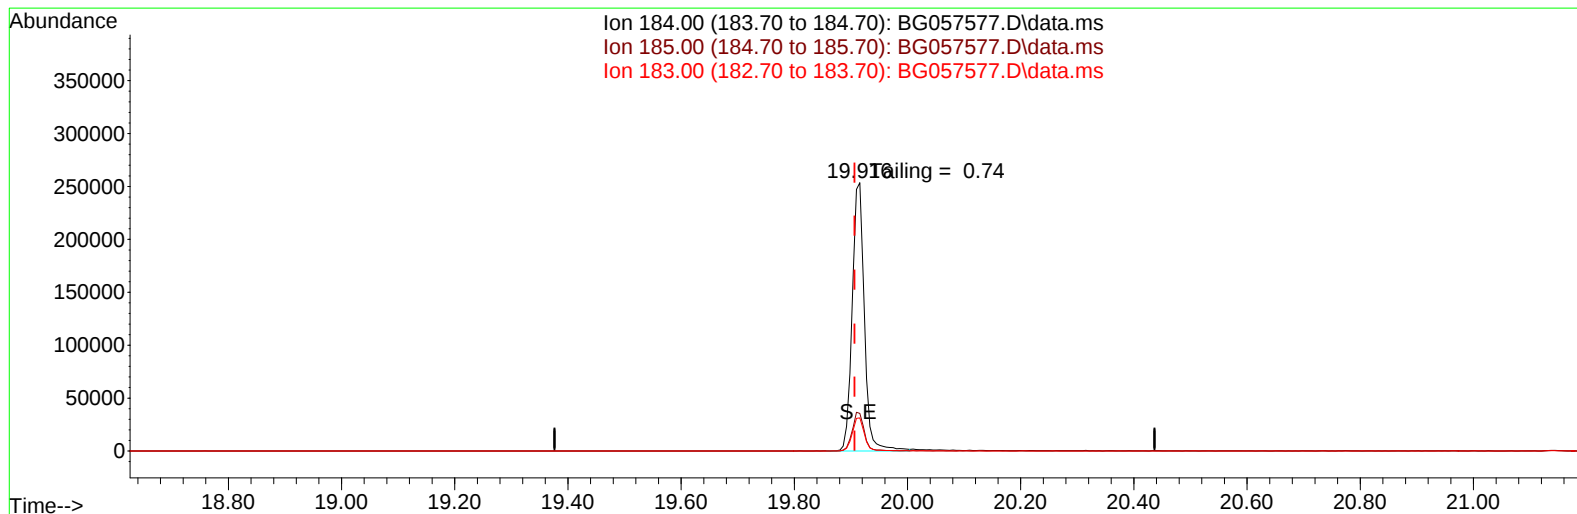

TIC: BG057577.D\data.ms

(77) Benzidine

19.916min (+ 0.010) 0.00 ng

response 382715

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.04
183.00	12.40	12.35
0.00	0.00	0.00