


Data Path : Z:\HPCHEM1\BNA_G\Data\BG052715\
Data File : BG017295.D
Acq On : 27 May 2015 9:51
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 13 16:12:13 2015

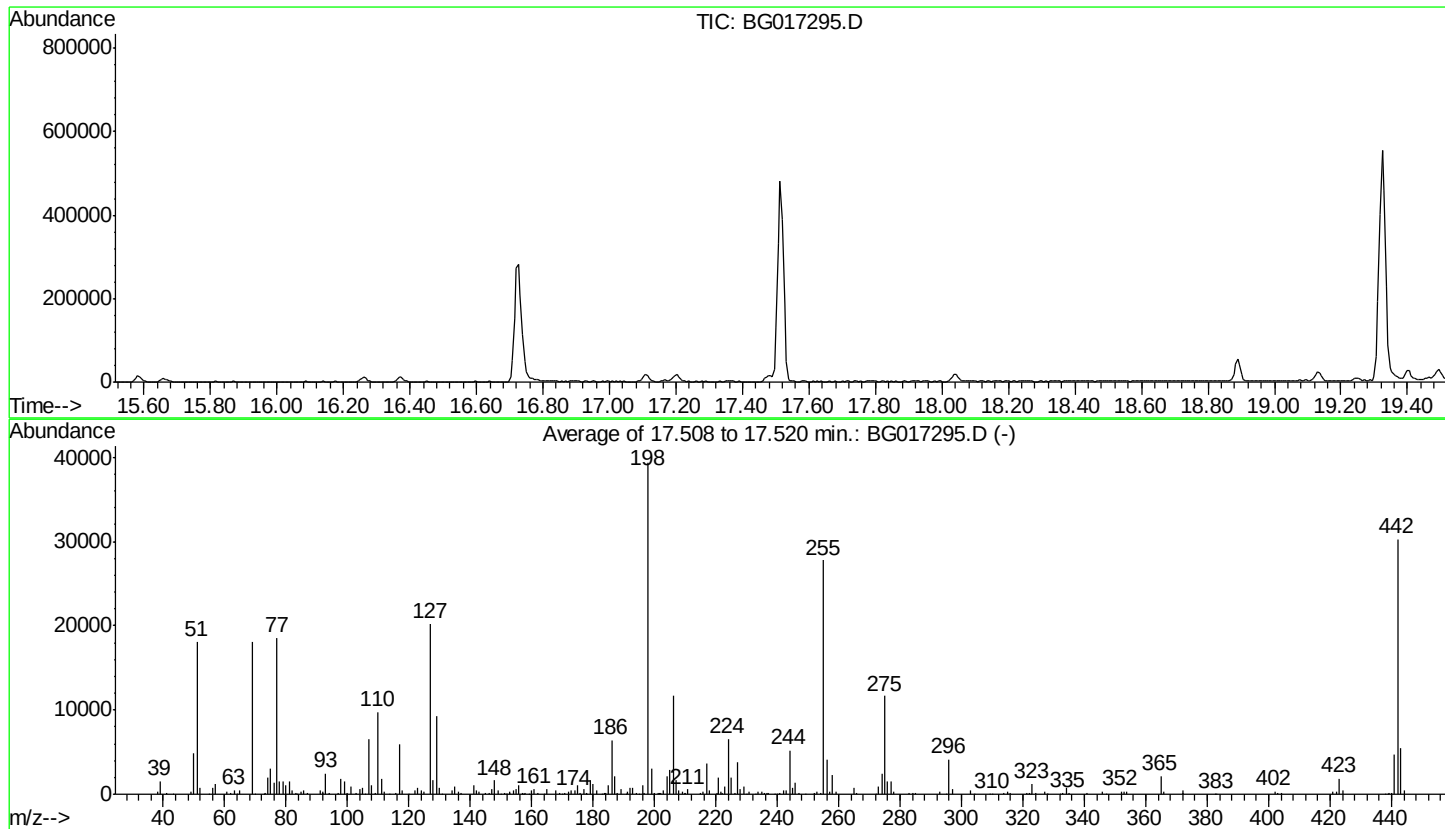

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	18088	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.8	18050	PASS
70	69	0.00	2	0.4	74	PASS
127	198	10	80	51.5	20282	PASS
197	198	0.00	2	0.3	113	PASS
198	198	100	100	100.0	39373	PASS
199	198	5	9	7.7	3029	PASS
275	198	10	60	29.7	11695	PASS
365	198	1	100	5.5	2161	PASS
441	442	0.01	24	15.6	4708	PASS
442	198	50	100	76.9	30272	PASS
443	442	15	24	18.3	5529	PASS