


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052715\
 Data File : BG017313.D
 Acq On : 27 May 2015 23:17
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 28 02:22:53 2015

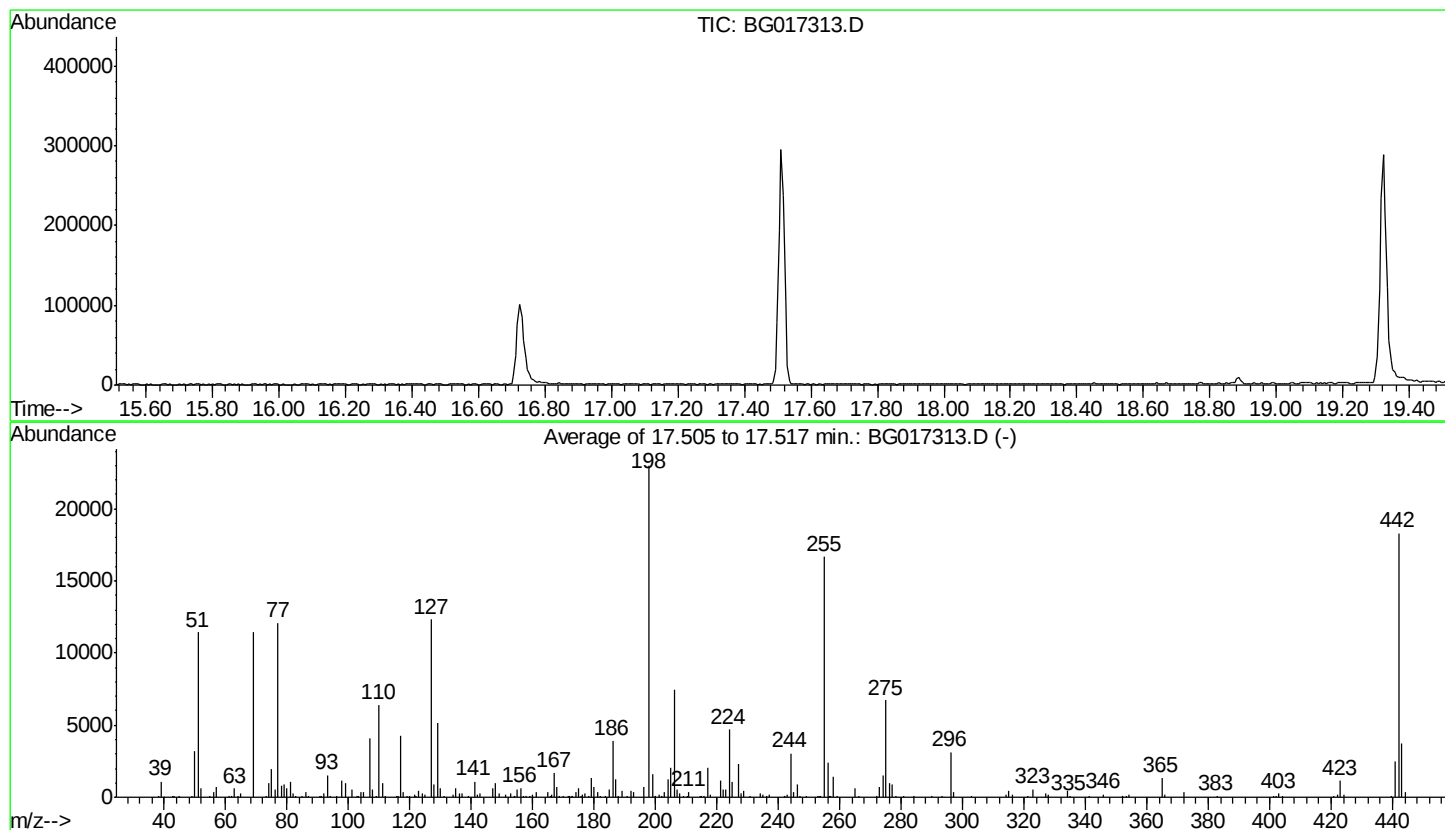

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.7	11425	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.7	11438	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.6	12323	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22997	PASS
199	198	5	9	6.9	1584	PASS
275	198	10	60	29.2	6723	PASS
365	198	1	100	5.8	1332	PASS
441	442	0.01	24	13.8	2527	PASS
442	198	50	100	79.6	18316	PASS
443	442	15	24	20.4	3741	PASS