
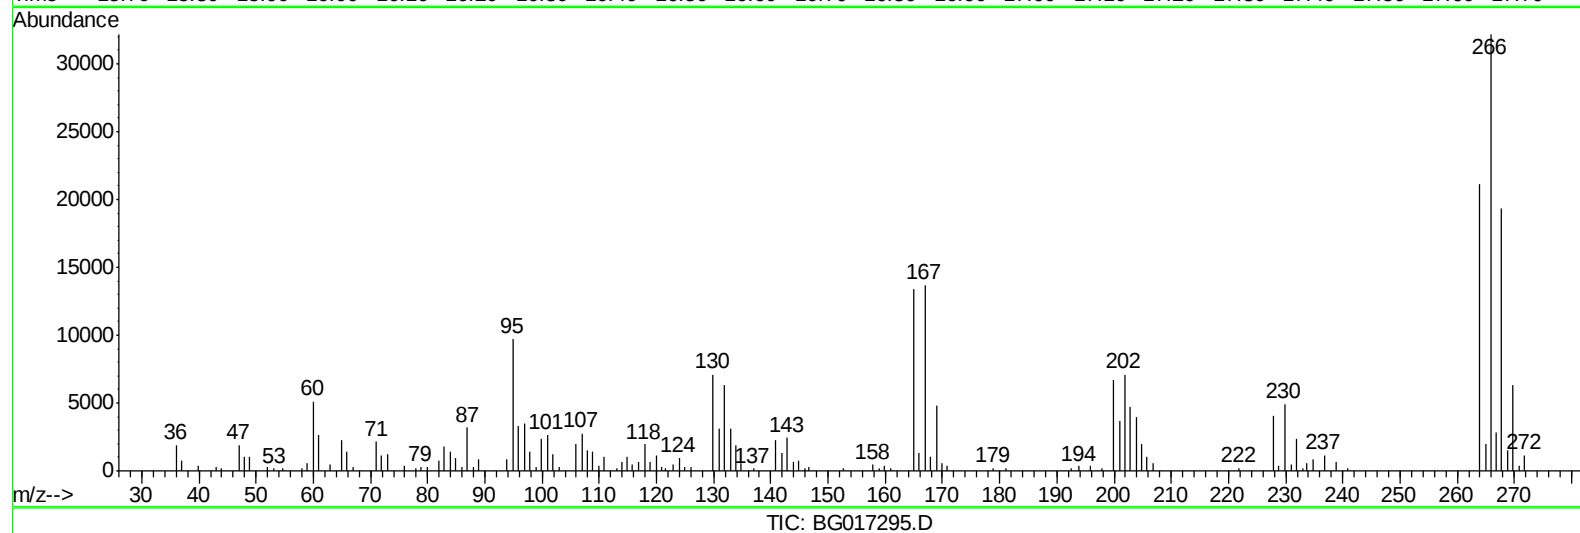


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052715\
Data File : BG017295.D
Acq On : 27 May 2015 9:51
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 06:42:32 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 28 02:22:53 2015
Response via : Initial Calibration

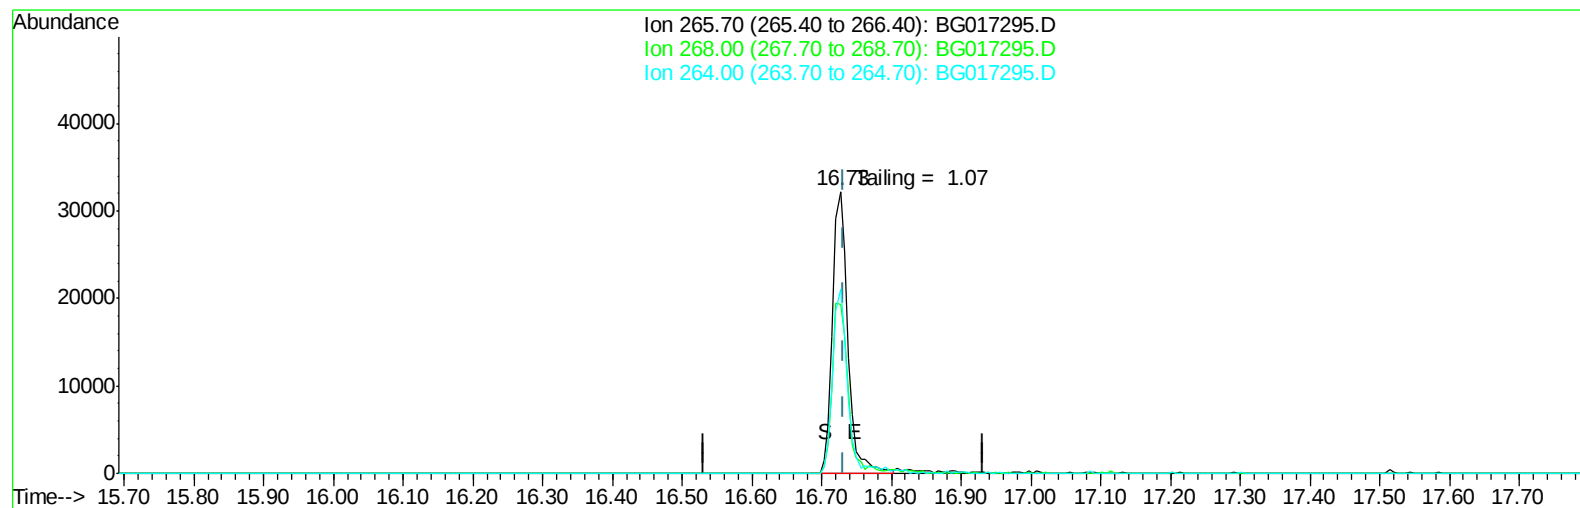

(69) Pentachlorophenol (C)



16.726min (-0.005) 2933.07ng

response 48825

Ion	Exp%	Act%
265.70	100	100
268.00	70.70	60.04
264.00	61.70	65.56
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052715\
Data File : BG017295.D
Acq On : 27 May 2015 9:51
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 06:42:32 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 28 02:22:53 2015
Response via : Initial Calibration

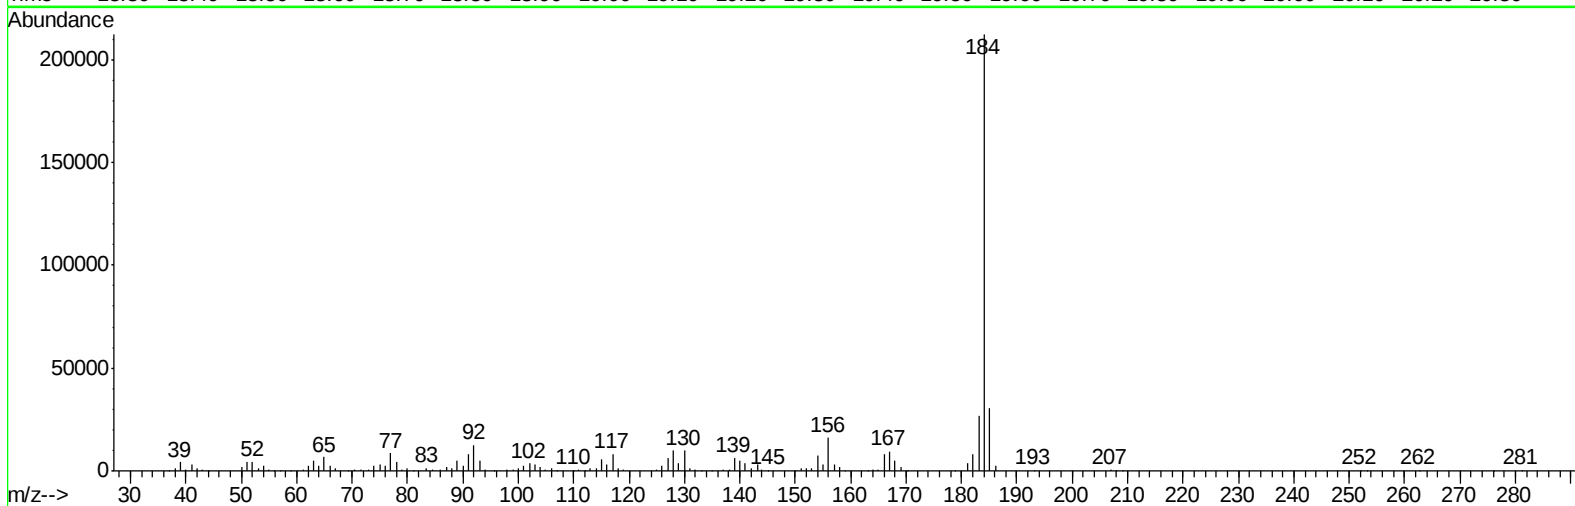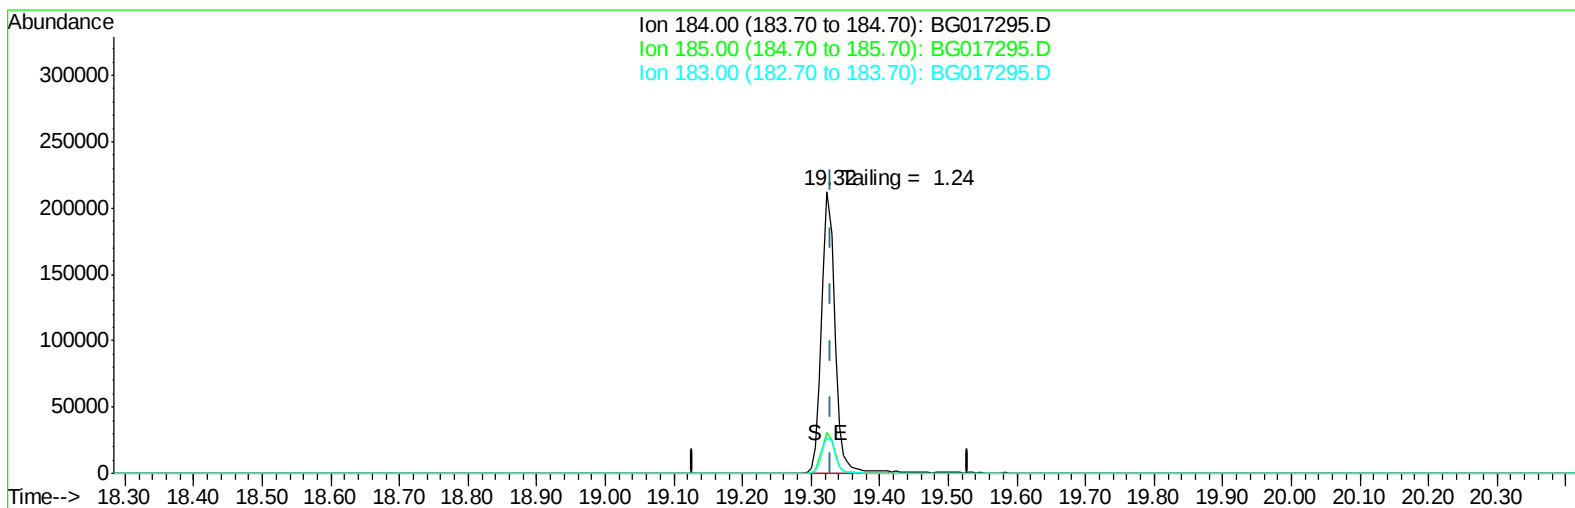

TIC: BG017295.D

(76) Benzidine

19.323min (-0.005) 25175.58ng

response 285226

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.38
183.00	14.30	12.66
0.00	0.00	0.00