

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052716\
 Data File : BG022107.D
 Acq On : 27 May 2016 15:08
 Operator : UM/SJ
 Sample : H3201-19RX
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZH5RX

Quant Time: May 27 18:43:55 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 27 18:06:31 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	44818	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	237767	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	132406	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.53	188	244939	20.00	ng/ul	0.00
75) Chrysene-d12	21.81	240	206459	20.00	ng/ul	0.00
83) Perylene-d12	25.14	264	204280	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	1273	1.48	ng/uL	0.00
5) Phenol-d5	7.32	99	2082	0.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	33729	15.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	1661	0.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	4043	1.18	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	29965	17.09	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	271	0.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.61	165	1456	0.43	ng/ul	0.01
29) 4-Chloroaniline-d4	11.11	131	83506	22.88	ng/ul	0.00
43) Dimethylphthalate-d6	14.17	166	116807	11.75	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	276892	19.94	ng/ul	0.00
51) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
57) Fluorene-d10	15.77	176	178141	19.13	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.63	188	242319	20.61	ng/ul	0.00
76) Pyrene-d10	19.90	212	236543	20.32	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.91	264	196862	20.77	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.22	163	26313	2.63	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052716\
Data File : BG022107.D
Acq On : 27 May 2016 15:08
Operator : UM/SJ
Sample : H3201-19RX
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCZH5RX

Quant Time: May 27 18:43:55 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 27 18:06:31 2016
Response via : Initial Calibration

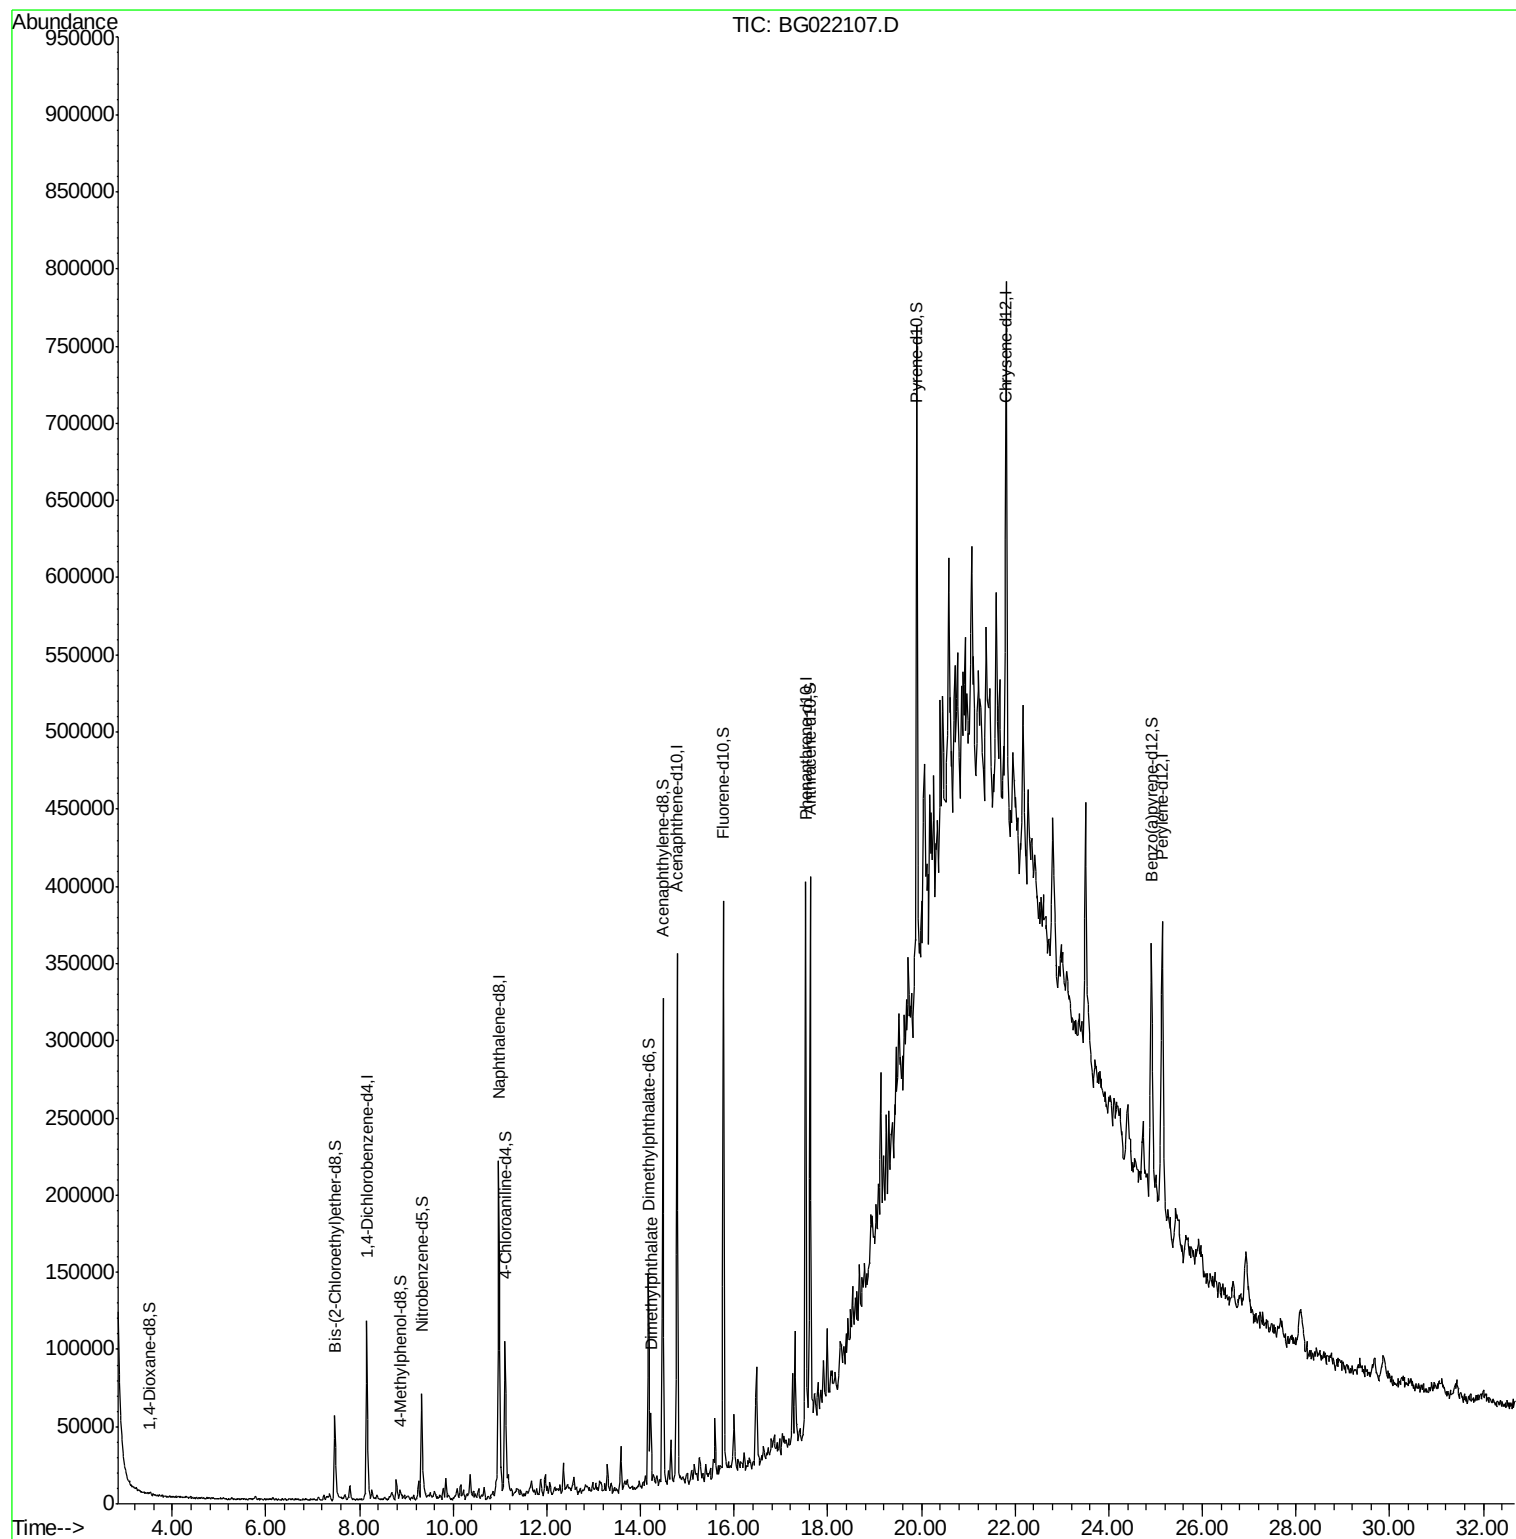

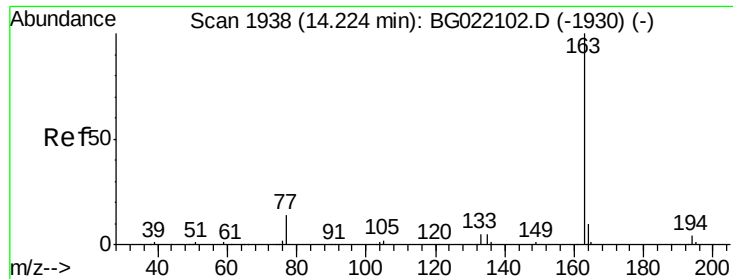

#44

Dimethylphthalate

Concen: 2.63 ng/ul

RT: 14.22 min Scan# 1937

Delta R.T. -0.01 min

Lab File: BG022107.D

Acq: 27 May 2016 15:08

Instrument :

BNA_G

ClientSampleId :

BCZH5RX

Tgt Ion:163 Resp: 26313

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2

164 10.6 8.8 13.2

