

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052716\
 Data File : BG022106.D
 Acq On : 27 May 2016 14:27
 Operator : UM/SJ
 Sample : PB90947BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.526	112	117	122	rBV3	6006	9012	0.86%	0.088%
2	3.920	181	184	188	rBV4	1358	1900	0.18%	0.018%
3	4.037	202	204	208	rVB4	1003	1117	0.11%	0.011%
4	4.296	243	248	251	rBV5	1650	3445	0.33%	0.033%
5	4.942	355	358	360	rBV3	724	1073	0.10%	0.010%
6	5.124	385	389	392	rBV4	799	1212	0.12%	0.012%
7	7.316	755	762	777	rBV	109986	231518	22.12%	2.249%
8	7.416	777	779	782	rVV2	1446	2029	0.19%	0.020%
9	7.469	782	788	802	rVV	96763	193744	18.51%	1.882%
10	7.563	802	804	809	rVB4	1747	2345	0.22%	0.023%
11	7.686	817	825	836	rBV	128681	256900	24.55%	2.496%
12	7.845	849	852	854	rVB3	1263	1323	0.13%	0.013%
13	8.156	897	905	919	rBV	90822	191353	18.29%	1.859%
14	8.867	1017	1026	1047	rBV	159290	342203	32.70%	3.325%
15	9.325	1095	1104	1121	rBV	113291	245526	23.46%	2.385%
16	10.054	1220	1228	1238	rBV	95073	201650	19.27%	1.959%
17	10.118	1238	1239	1243	rVB4	2194	1949	0.19%	0.019%
18	10.600	1313	1321	1335	rBV	153992	337171	32.22%	3.276%
19	10.806	1352	1356	1360	rBV2	911	1549	0.15%	0.015%
20	10.976	1376	1385	1395	rBV	169367	348003	33.25%	3.381%
21	11.106	1399	1407	1423	rBV	150802	344156	32.89%	3.344%
22	12.551	1648	1653	1655	rBV3	2184	3194	0.31%	0.031%
23	12.569	1655	1656	1660	rVB	1644	1230	0.12%	0.012%
24	13.650	1835	1840	1845	rBV2	874	1390	0.13%	0.014%
25	14.173	1922	1929	1941	rBV	337944	547401	52.31%	5.318%
26	14.478	1971	1981	1992	rBV	453971	779297	74.47%	7.571%
27	14.619	2002	2005	2012	rVB3	889	1864	0.18%	0.018%
28	14.778	2025	2032	2041	rBV2	282258	509744	48.71%	4.952%
29	14.995	2063	2069	2084	rBV	55747	159466	15.24%	1.549%
30	15.771	2189	2201	2215	rBV	555616	940244	89.85%	9.135%
31	15.888	2215	2221	2229	rBV	87264	150986	14.43%	1.467%
32	16.006	2236	2241	2247	rVB2	5475	8623	0.82%	0.084%
33	17.522	2493	2499	2509	rBV	318804	552602	52.81%	5.369%
34	17.621	2509	2516	2539	rVV2	559027	970791	92.77%	9.432%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052716\
 Data File : BG022106.D
 Acq On : 27 May 2016 14:27
 Operator : UM/SJ
 Sample : PB90947BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

35	17.768	2539	2541	2543	rVV3	1904	2165	0.21%	0.021%
36	17.798	2543	2546	2548	rVV3	1233	1767	0.17%	0.017%
37	17.821	2548	2550	2553	rVV3	1029	1237	0.12%	0.012%
38	18.097	2594	2597	2600	rBV3	1350	1801	0.17%	0.017%
39	18.397	2646	2648	2651	rVB2	2207	1926	0.18%	0.019%
40	18.432	2653	2654	2657	rBV	1296	1139	0.11%	0.011%
41	18.614	2683	2685	2687	rBV3	1013	1198	0.11%	0.012%
42	18.644	2689	2690	2694	rBV4	1687	1832	0.18%	0.018%
43	18.873	2725	2729	2730	rBV3	991	1393	0.13%	0.014%
44	18.943	2738	2741	2742	rVV3	1397	1187	0.11%	0.012%
45	18.961	2742	2744	2746	rVB3	1431	1189	0.11%	0.012%
46	19.020	2752	2754	2756	rBV2	1445	1095	0.10%	0.011%
47	19.073	2761	2763	2765	rVV2	1601	1304	0.12%	0.013%
48	19.114	2768	2770	2772	rVB3	1496	1181	0.11%	0.011%
49	19.155	2772	2777	2778	rBV3	2290	3053	0.29%	0.030%
50	19.255	2792	2794	2796	rVB3	1665	1390	0.13%	0.014%
51	19.290	2796	2800	2801	rBV4	1743	2496	0.24%	0.024%
52	19.343	2803	2809	2810	rVV5	1097	2134	0.20%	0.021%
53	19.449	2824	2827	2828	rBV3	2043	1821	0.17%	0.018%
54	19.537	2838	2842	2848	rBV2	6783	14708	1.41%	0.143%
55	19.601	2851	2853	2855	rVB3	1966	1468	0.14%	0.014%
56	19.795	2880	2886	2888	rBV3	6951	10965	1.05%	0.107%
57	19.901	2897	2904	2915	rBV	655459	1046494	100.00%	10.167%
58	20.424	2991	2993	2997	rBV5	3866	4724	0.45%	0.046%
59	21.805	3221	3228	3239	rVB	258236	509429	48.68%	4.949%
60	23.661	3542	3544	3545	rBV2	6544	4023	0.38%	0.039%
61	24.907	3745	3756	3774	rVB2	251013	819395	78.30%	7.961%
62	25.130	3785	3794	3807	rVB3	152263	504171	48.18%	4.898%


Sum of corrected areas: 10292695

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052716\
Data File : BG022106.D
Acq On : 27 May 2016 14:27
Operator : UM/SJ
Sample : PB90947BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK47

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

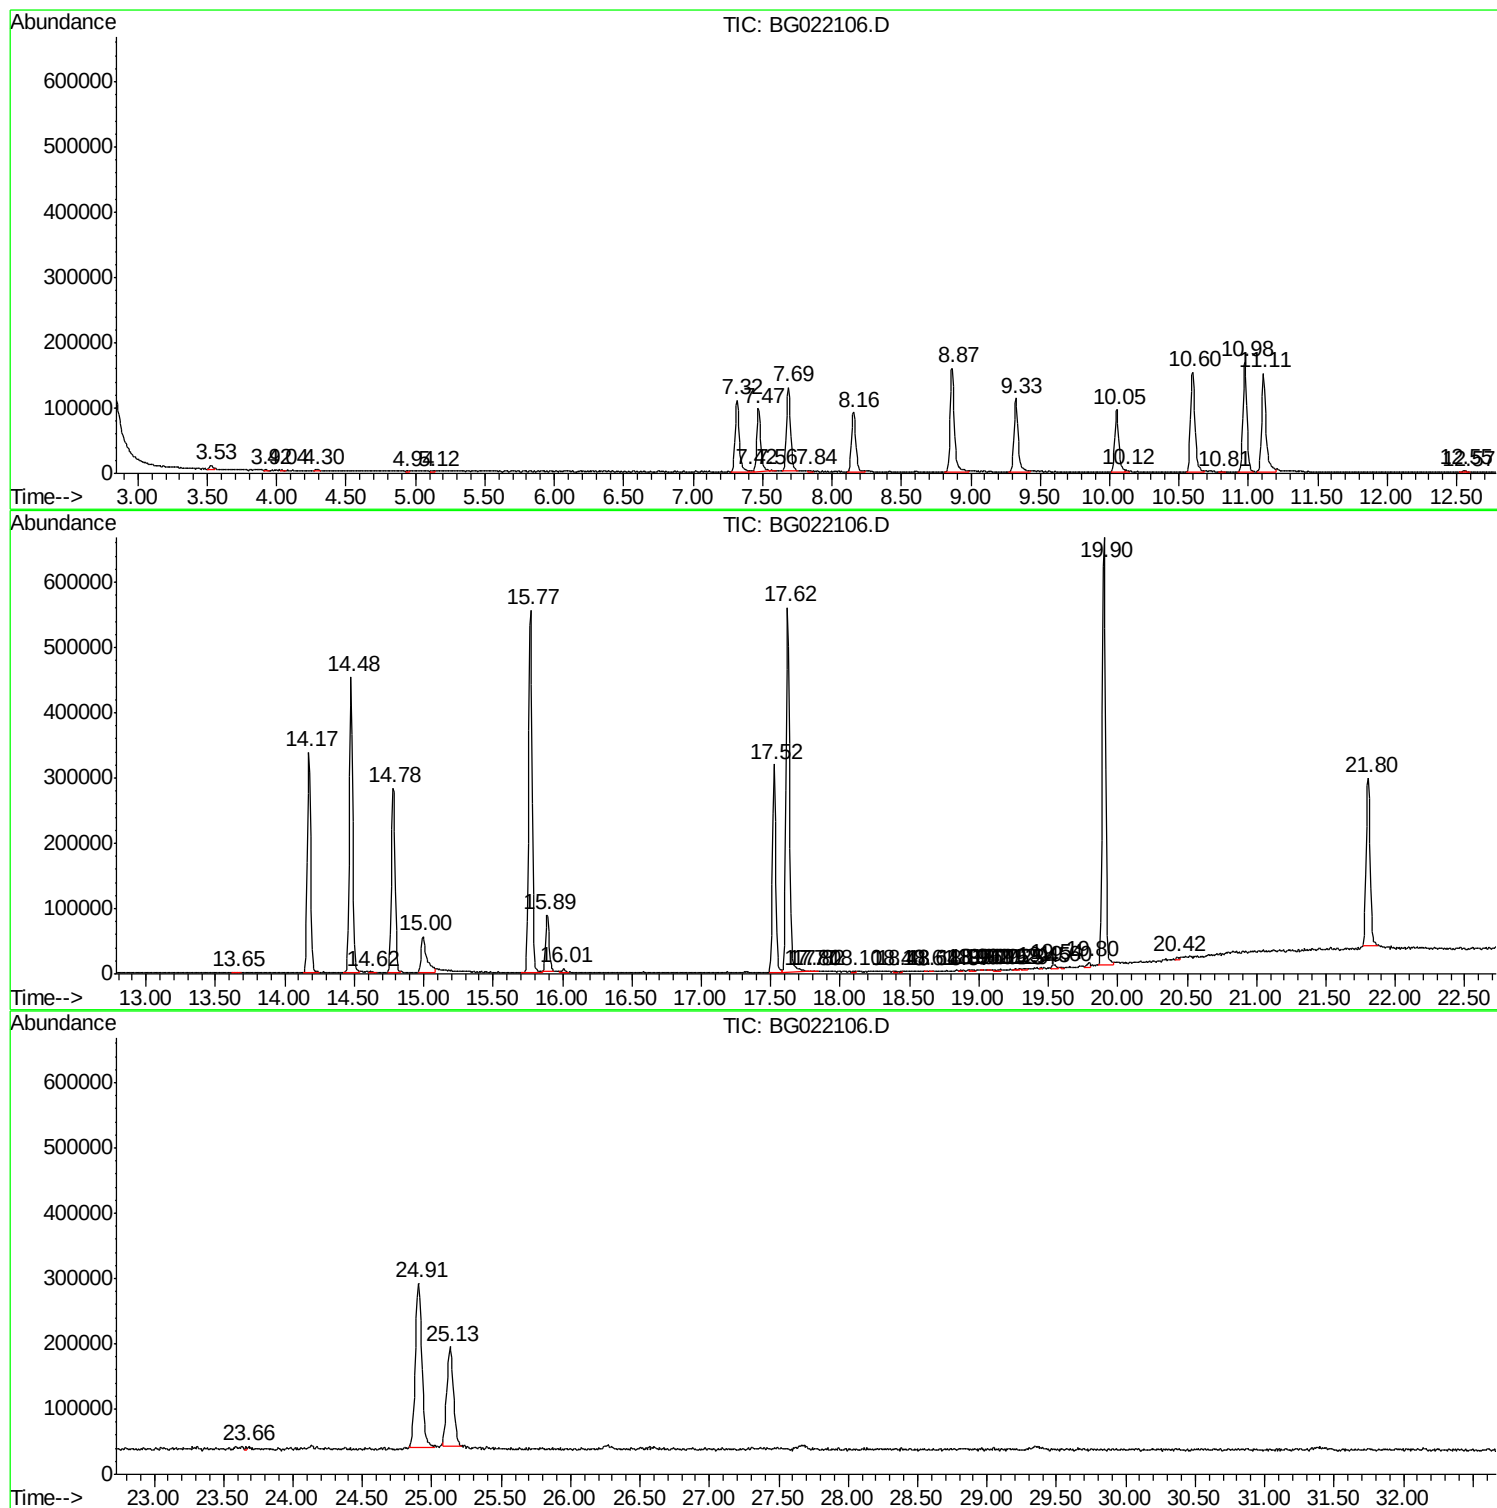

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052716\
Data File : BG022106.D
Acq On : 27 May 2016 14:27
Operator : UM/SJ
Sample : PB90947BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK47

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052716\
Data File : BG022106.D
Acq On : 27 May 2016 14:27
Operator : UM/SJ
Sample : PB90947BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK47

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc