
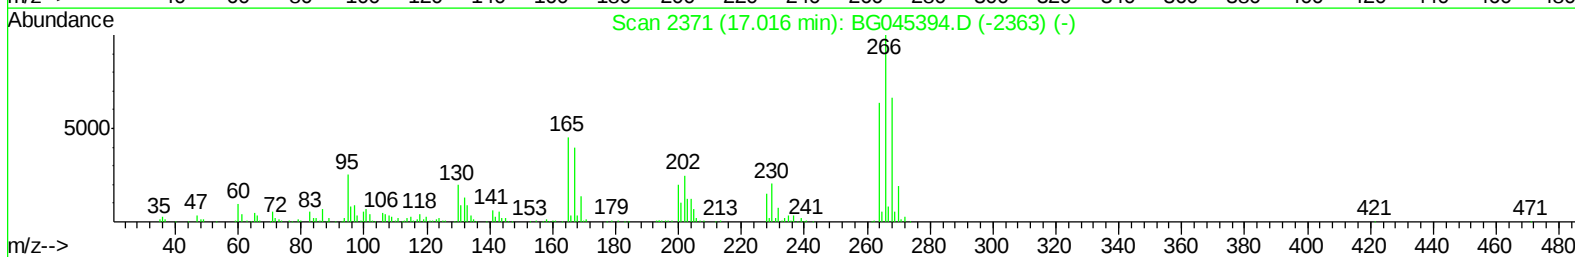
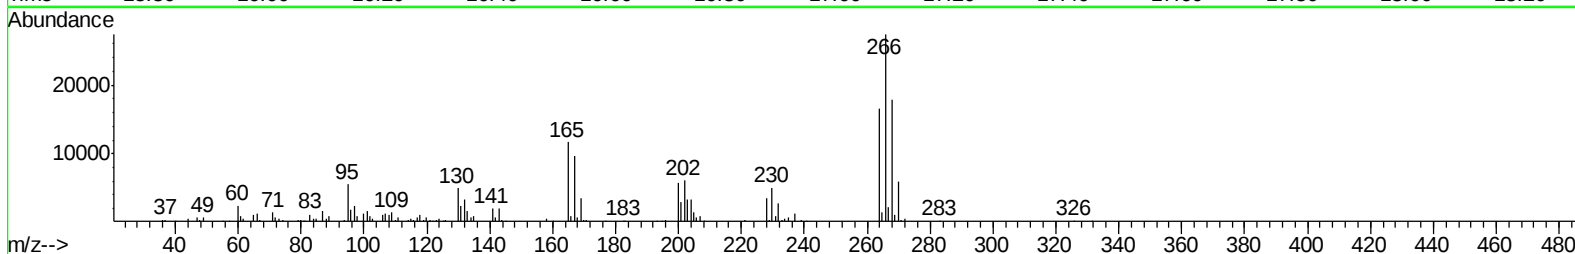


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG052720\  
 Data File : BG045472.D  
 Acq On : 27 May 2020 12:12  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 02:32:55 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed May 27 13:40:45 2020  
 Response via : Initial Calibration

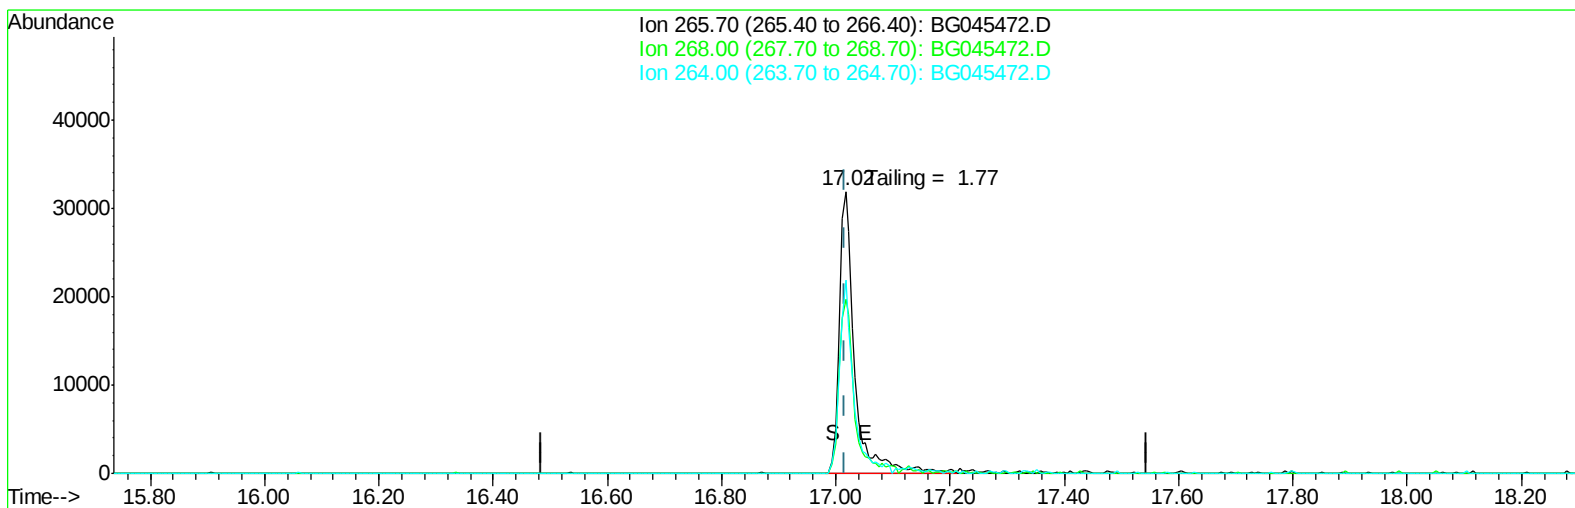

TIC: BG045472.D

(70) Pentachlorophenol (C)




17.017min (+0.000) 18882.25ng

response 57408

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 66.50 | 61.77 |
| 264.00 | 63.70 | 68.67 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG052720\  
 Data File : BG045472.D  
 Acq On : 27 May 2020 12:12  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 02:32:55 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed May 27 13:40:45 2020  
 Response via : Initial Calibration

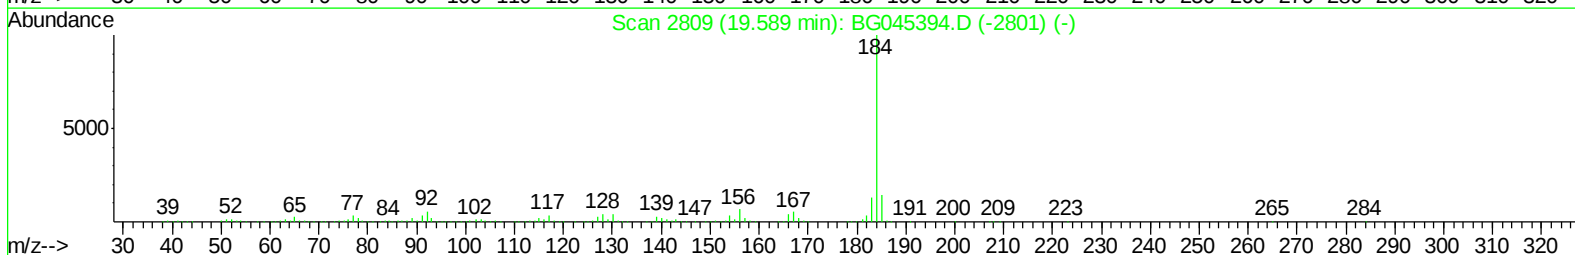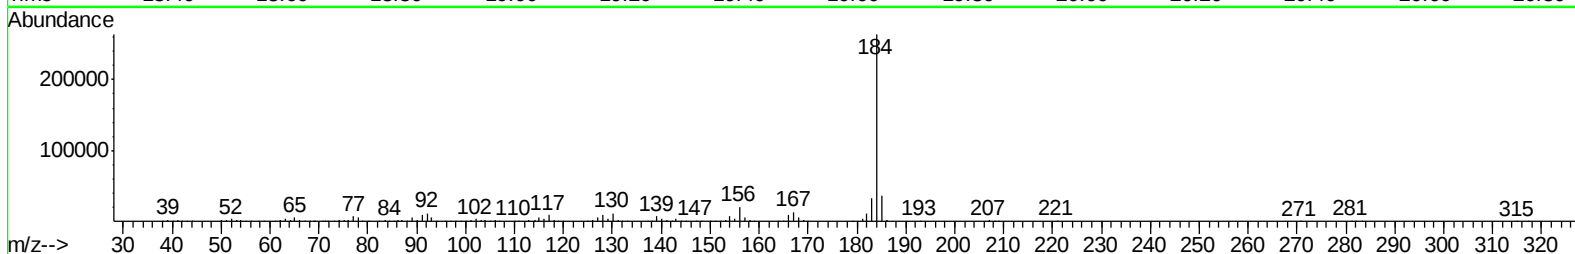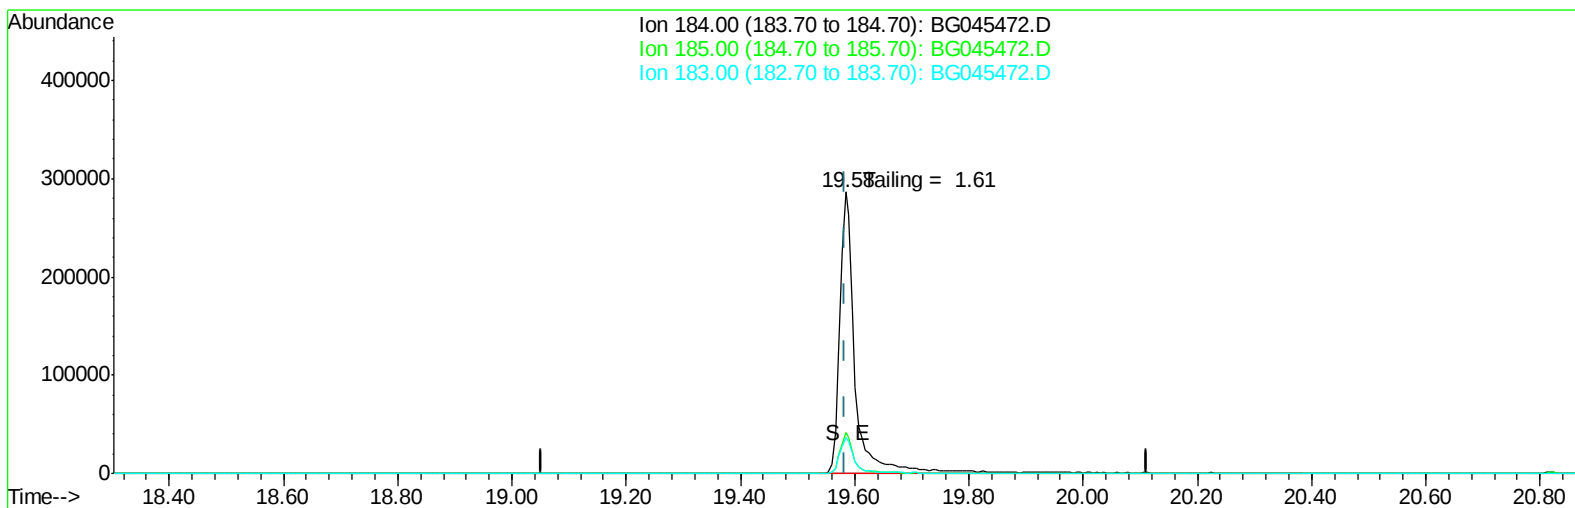

TIC: BG045472.D

(77) Benzidine

19.584min (+0.000) 274041.25ng

response 515671

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.60 | 14.72 |
| 183.00 | 12.80 | 12.86 |
| 0.00   | 0.00  | 0.00  |