
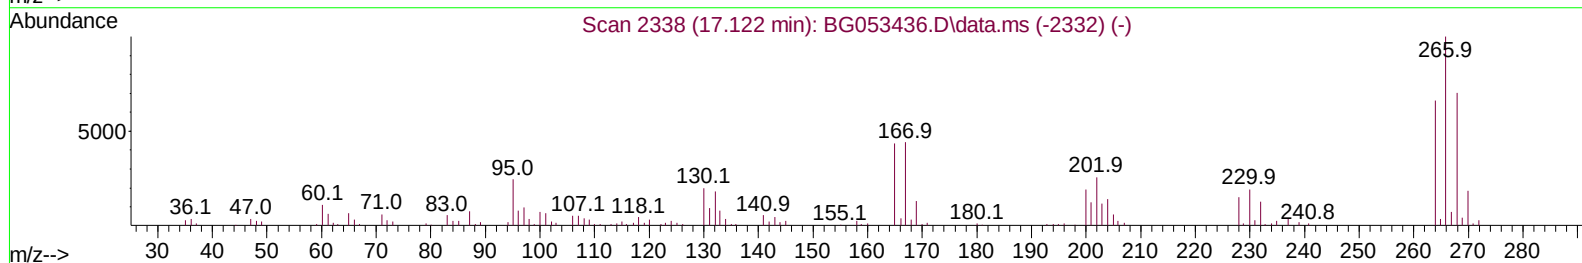
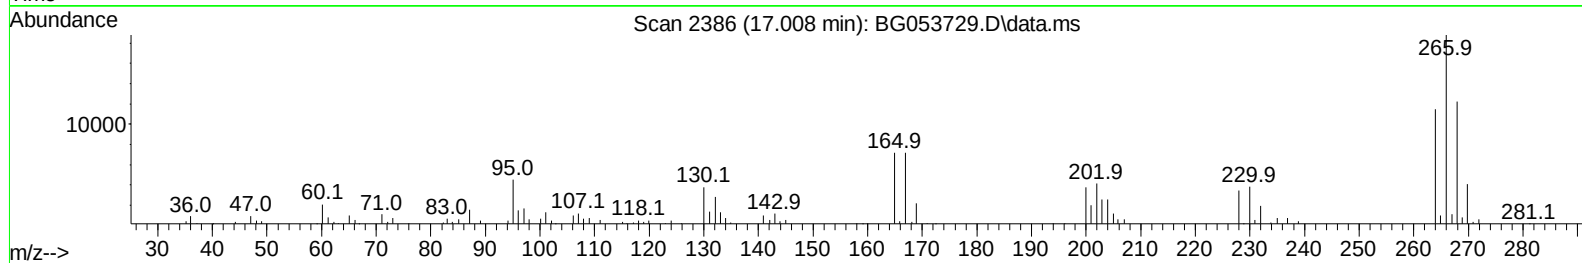


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053729.D
Acq On : 27 May 2022 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 06:39:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

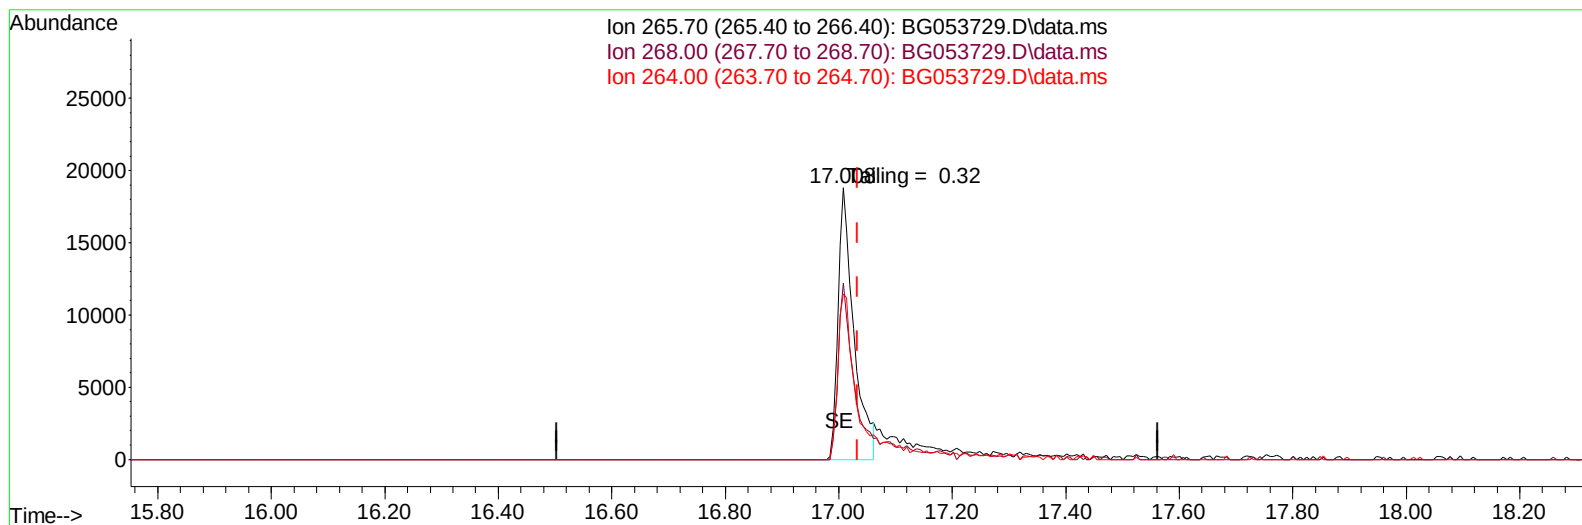

TIC: BG053729.D\data.ms

(70) Pentachlorophenol (C)




17.008min (-0.025) 18456.81 ng

response 38864

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.07
264.00	66.20	61.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053729.D
Acq On : 27 May 2022 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 11:57:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

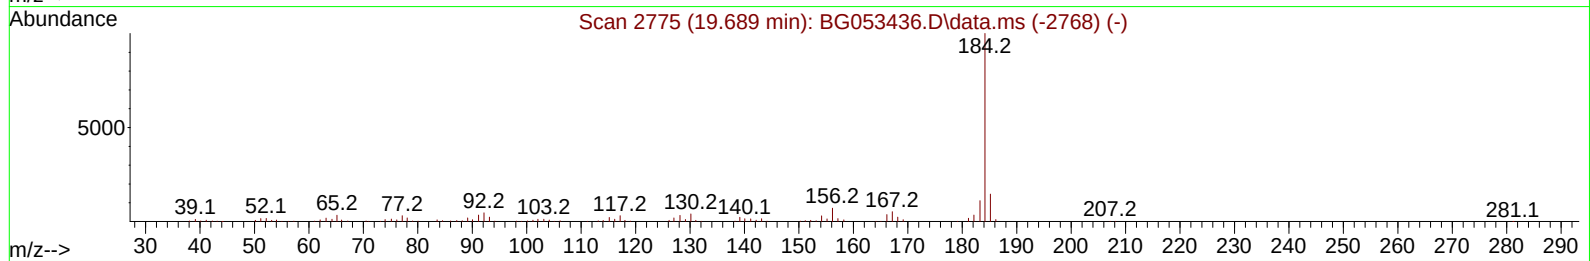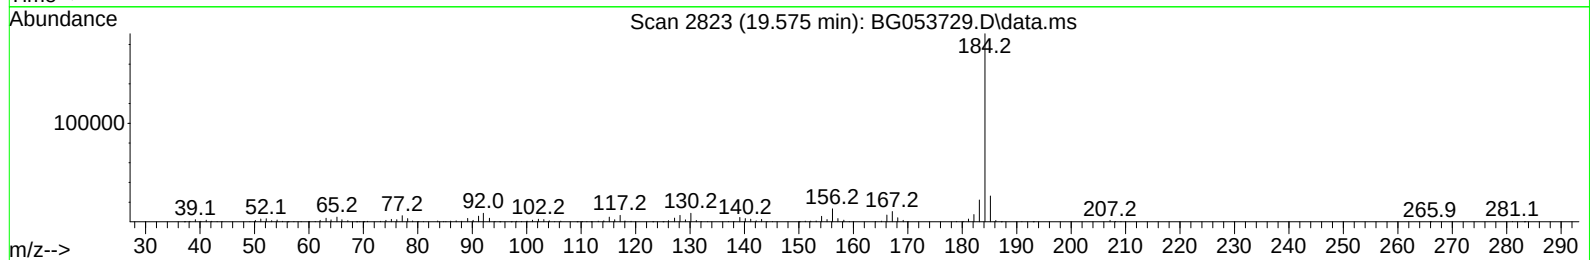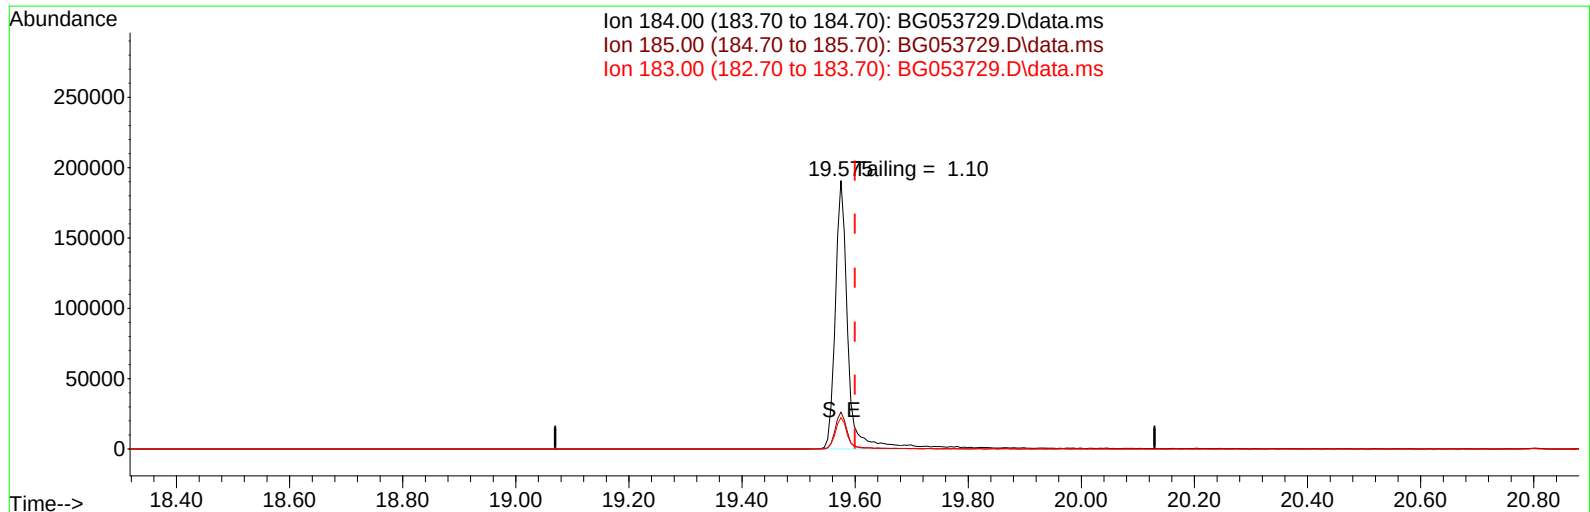

TIC: BG053729.D\data.ms

(77) Benzidine

19.575min (-0.025) 0.00 ng

response 287731

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.79
183.00	11.10	11.68
0.00	0.00	0.00