

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053737.D
 Acq On : 27 May 2022 17:31
 Operator : CG/JU
 Sample : N3072-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PSC-124030

Quant Time: May 28 01:58:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 25 15:11:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	20880	20.000	ng	-0.03
21) Naphthalene-d8	10.759	136	84900	20.000	ng	-0.04
39) Acenaphthene-d10	14.595	164	64662	20.000	ng	-0.03
64) Phenanthrene-d10	17.339	188	160705	20.000	ng	-0.03
76) Chrysene-d12	21.604	240	159727	20.000	ng	-0.03
86) Perylene-d12	24.782	264	155915	20.000	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.519	112	138812	112.827	ng	-0.03
7) Phenol-d6	7.129	99	205496	110.057	ng	-0.03
23) Nitrobenzene-d5	9.115	82	141829	71.112	ng	-0.04
42) 2,4,6-Tribromophenol	16.087	330	111706	117.130	ng	-0.03
45) 2-Fluorobiphenyl	13.215	172	282150	63.762	ng	-0.03
79) Terphenyl-d14	19.953	244	527091	61.461	ng	-0.02
Target Compounds						
75) Fluoranthene	19.395	202	23790	2.248	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053737.D
Acq On : 27 May 2022 17:31
Operator : CG/JU
Sample : N3072-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PSC-124030

Quant Time: May 28 01:58:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration




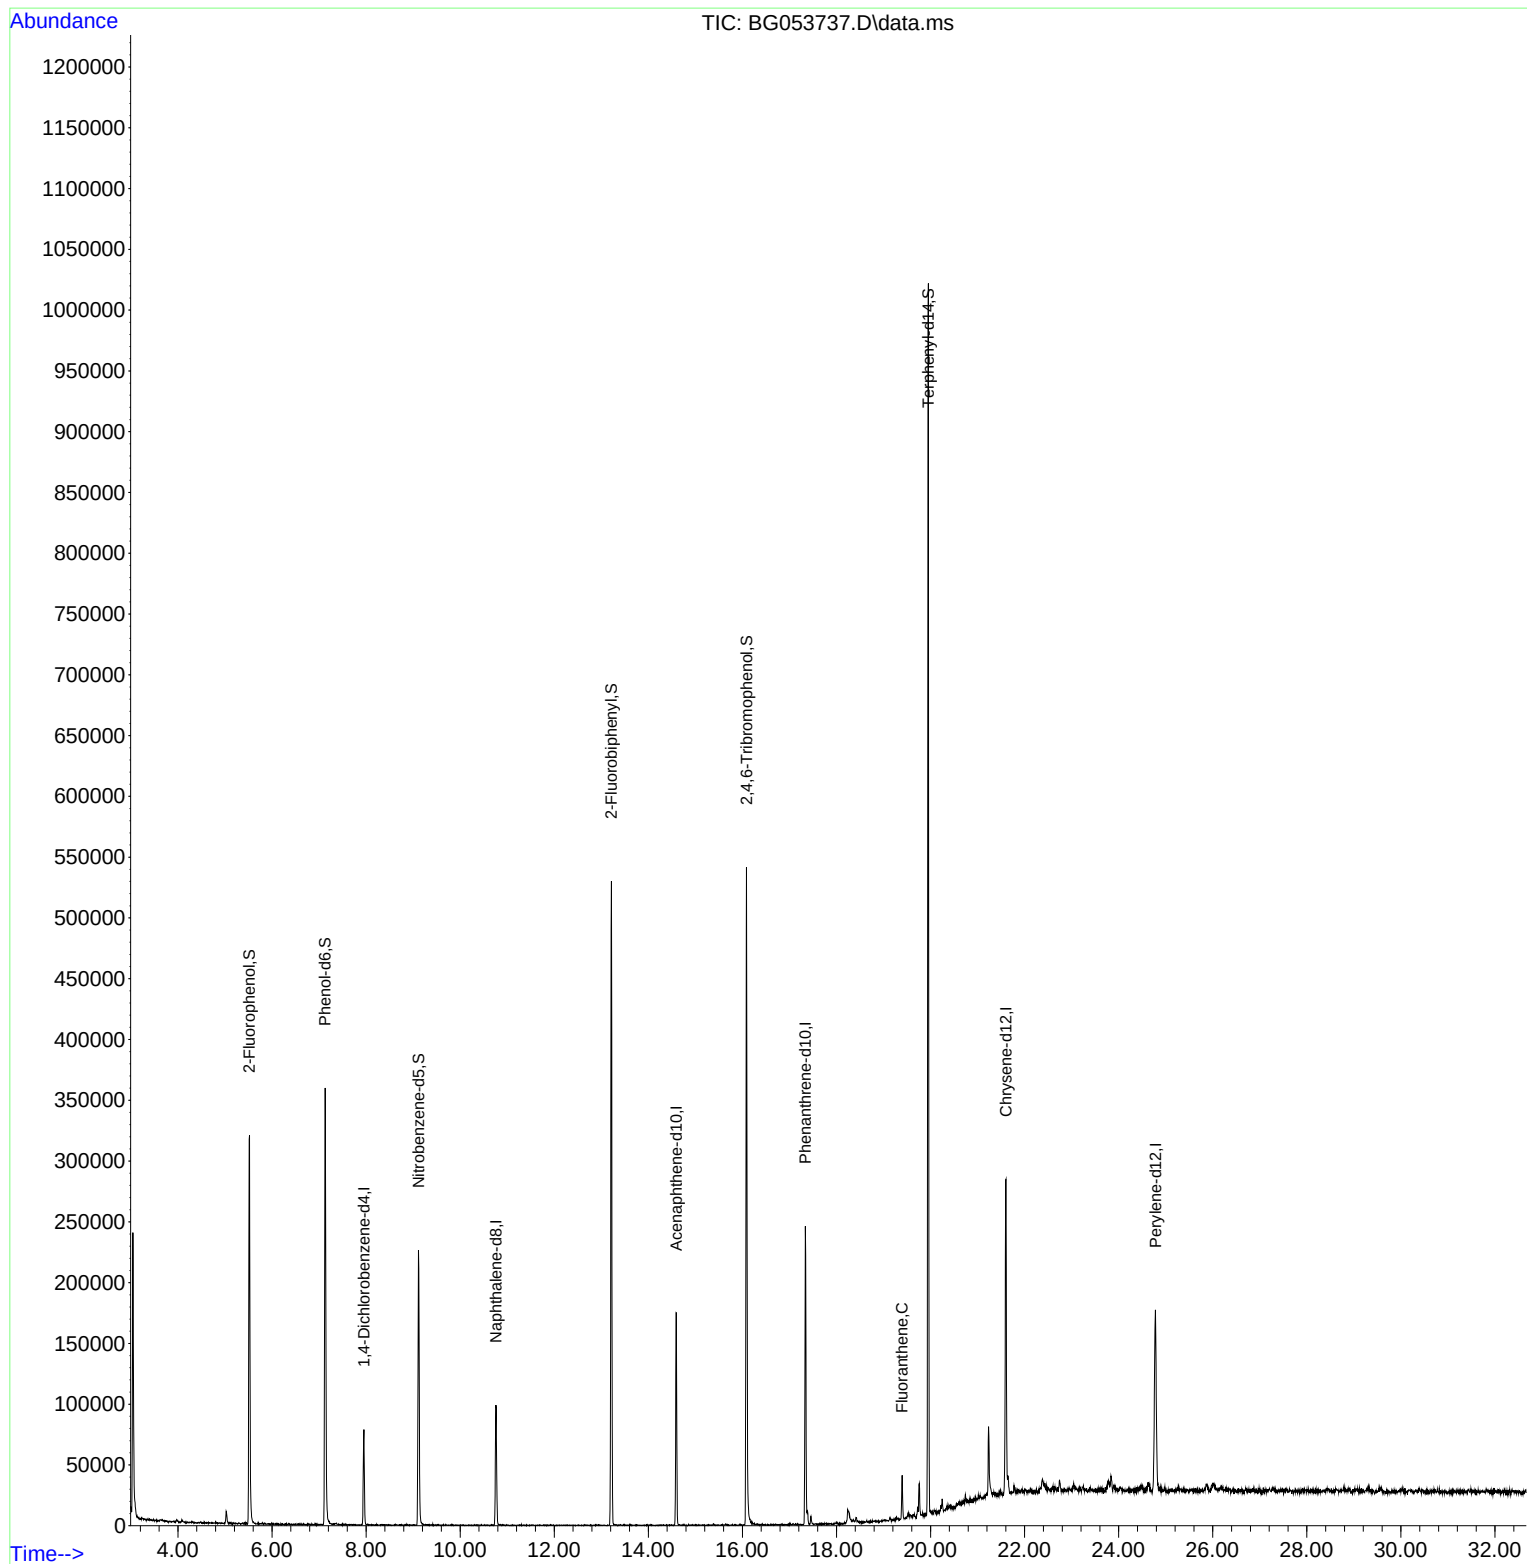




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.951 min Scan# 84
Delta R.T. -0.035 min
Lab File: BG053737.D
Acq: 27 May 2022 17:31




Instrument :
BNA_G
ClientSampleId :
PSC-124030


Tgt Ion:152 Resp: 20880
Ion Ratio Lower Upper
152 100
150 161.7 131.6 197.4
115 65.9 50.9 76.3

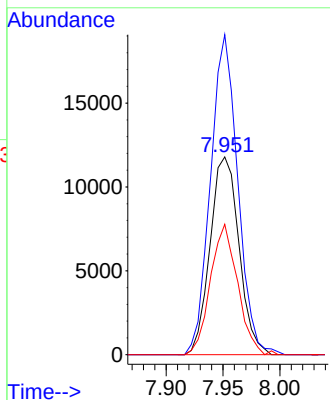

#5
2-Fluorophenol
Concen: 112.827 ng
RT: 5.519 min Scan# 431
Delta R.T. -0.035 min
Lab File: BG053737.D
Acq: 27 May 2022 17:31

Tgt Ion:112 Resp: 138812
Ion Ratio Lower Upper
112 100
64 68.6 55.1 82.7
63 38.3 30.4 45.6


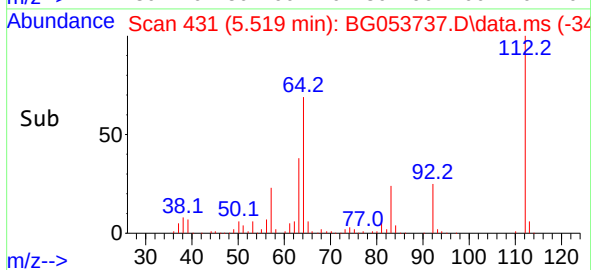
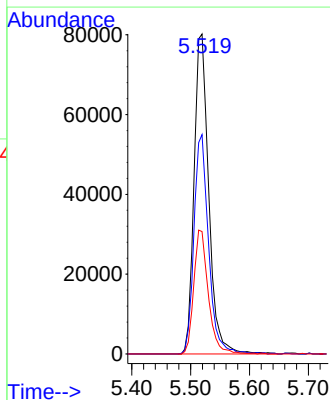





#7
Phenol-d6
Concen: 110.057 ng
RT: 7.129 min Scan# 705
Delta R.T. -0.035 min
Lab File: BG053737.D
Acq: 27 May 2022 17:31




Instrument :
BNA_G
ClientSampleId :
PSC-124030


Tgt Ion: 99 Resp: 205496
Ion Ratio Lower Upper
99 100
42 20.7 17.0 25.6
71 42.9 33.8 50.8

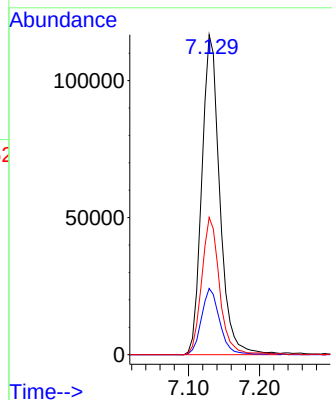

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.759 min Scan# 1323
Delta R.T. -0.041 min
Lab File: BG053737.D
Acq: 27 May 2022 17:31

Tgt Ion:136 Resp: 84900
Ion Ratio Lower Upper
136 100
137 11.8 8.5 12.7
54 8.7 7.4 11.2
68 7.0 4.9 7.3


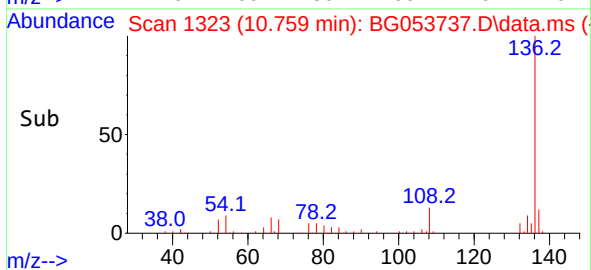
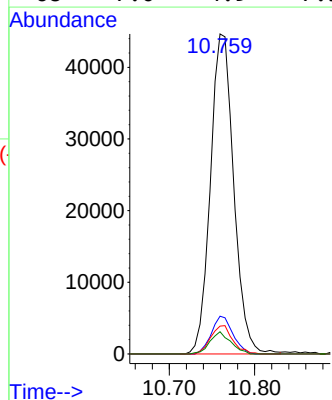





#23
Nitrobenzene-d5
Concen: 71.112 ng
RT: 9.115 min Scan# 10
Delta R.T. -0.041 min
Lab File: BG053737.D
Acq: 27 May 2022 17:31




Instrument :
BNA_G
ClientSampleId :
PSC-124030


Tgt Ion: 82 Resp: 141829
Ion Ratio Lower Upper
82 100
128 37.0 27.9 41.9
54 53.5 41.2 61.8

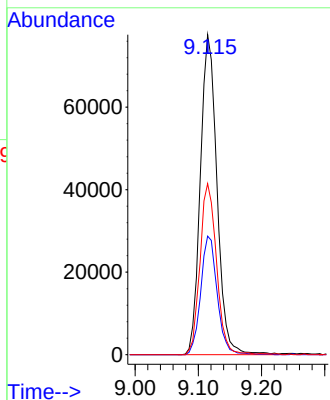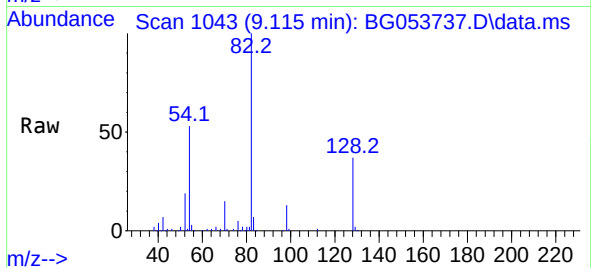

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.595 min Scan# 1976
Delta R.T. -0.029 min
Lab File: BG053737.D
Acq: 27 May 2022 17:31

Tgt Ion:164 Resp: 64662
Ion Ratio Lower Upper
164 100
162 102.4 82.3 123.5
160 41.4 34.2 51.2


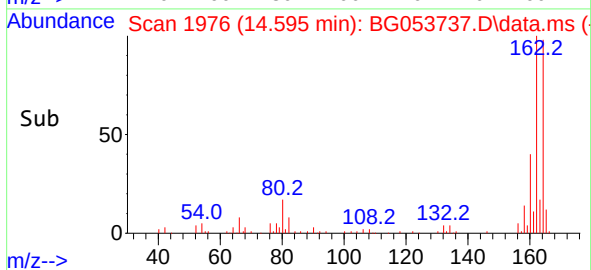
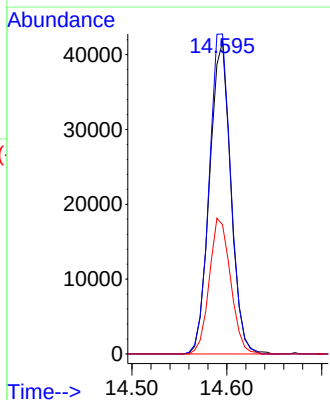





#42
2,4,6-Tribromophenol
Concen: 117.130 ng
RT: 16.087 min Scan# 2183
Delta R.T. -0.029 min
Lab File: BG053737.D
Acq: 27 May 2022 17:31




Instrument :
BNA_G
ClientSampleId :
PSC-124030


Tgt Ion:330 Resp: 111706
Ion Ratio Lower Upper
330 100
332 97.2 76.0 114.0
141 33.3 27.1 40.7

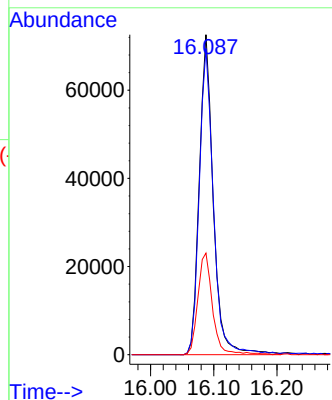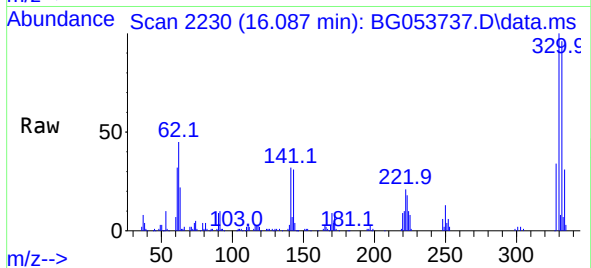

#45
2-Fluorobiphenyl
Concen: 63.762 ng
RT: 13.215 min Scan# 1741
Delta R.T. -0.029 min
Lab File: BG053737.D
Acq: 27 May 2022 17:31

Tgt Ion:172 Resp: 282150
Ion Ratio Lower Upper
172 100
171 35.2 28.5 42.7
170 21.7 18.9 28.3


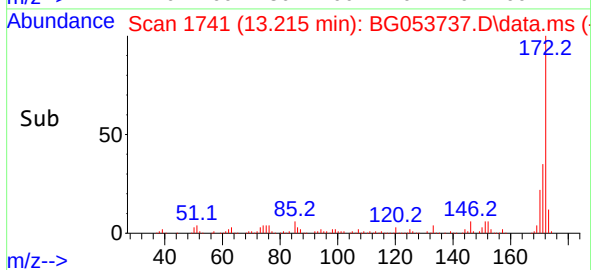
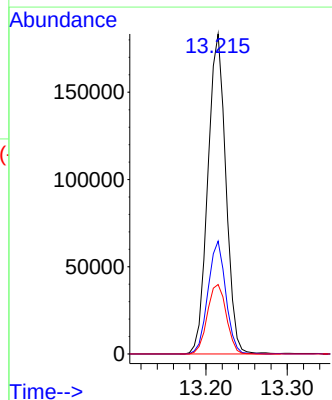





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.339 min Scan# 24
Delta R.T. -0.035 min
Lab File: BG053737.D
Acq: 27 May 2022 17:31




Instrument :
BNA_G
ClientSampleId :
PSC-124030


Tgt Ion:188 Resp: 160705
Ion Ratio Lower Upper
188 100
94 7.3 5.4 8.0
80 7.7 6.8 10.2

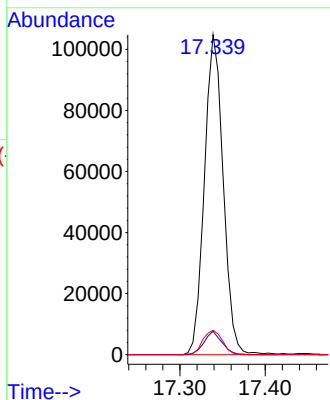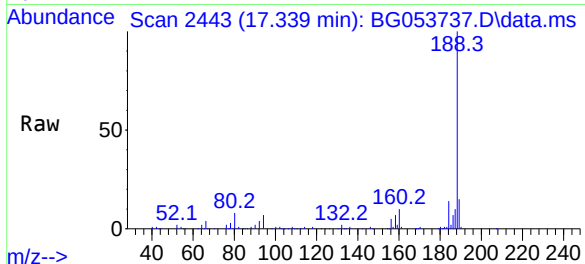

#75
Fluoranthene
Concen: 2.248 ng
RT: 19.395 min Scan# 2793
Delta R.T. -0.029 min
Lab File: BG053737.D
Acq: 27 May 2022 17:31

Tgt Ion:202 Resp: 23790
Ion Ratio Lower Upper
202 100
101 7.6 0.0 26.9
203 15.5 0.0 37.2


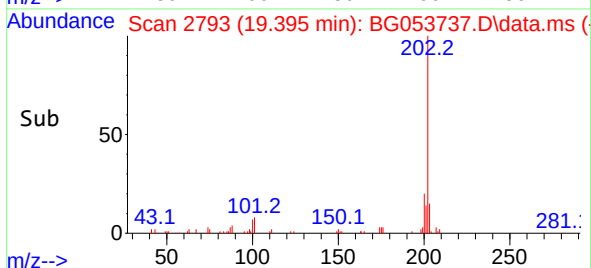
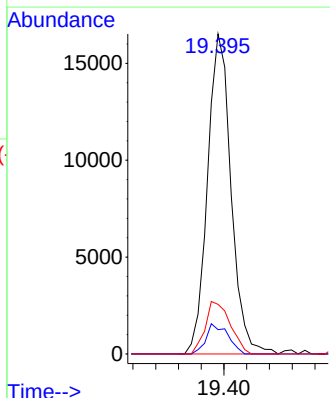
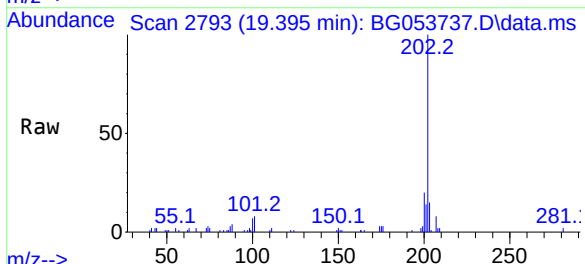




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.604 min Scan# 31
Delta R.T. -0.035 min
Lab File: BG053737.D
Acq: 27 May 2022 17:31




Instrument :
BNA_G
ClientSampleId :
PSC-124030


Tgt Ion:240 Resp: 159727
Ion Ratio Lower Upper
240 100
120 5.6 4.6 7.0
236 24.5 20.2 30.4

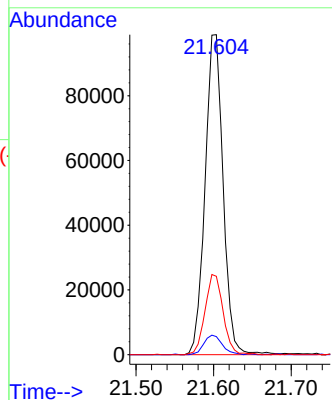

#79
Terphenyl-d14
Concen: 61.461 ng
RT: 19.953 min Scan# 2888
Delta R.T. -0.023 min
Lab File: BG053737.D
Acq: 27 May 2022 17:31


Tgt Ion:244 Resp: 527091
Ion Ratio Lower Upper
244 100
212 7.6 6.5 9.7
122 5.9 5.0 7.4

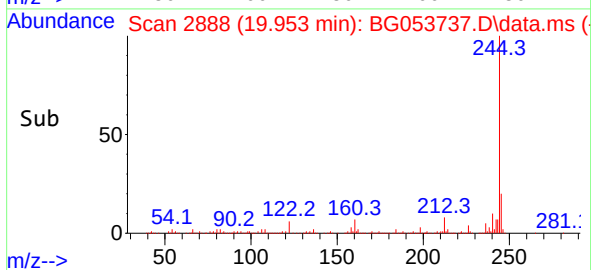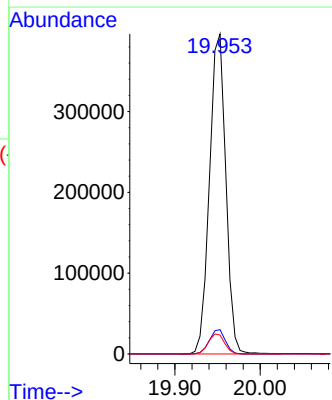

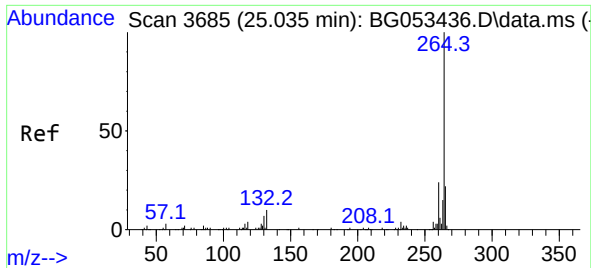

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.782 min Scan# 31
 Delta R.T. -0.058 min
 Lab File: BG053737.D
 Acq: 27 May 2022 17:31

Instrument :
 BNA_G
 ClientSampleId :
 PSC-124030

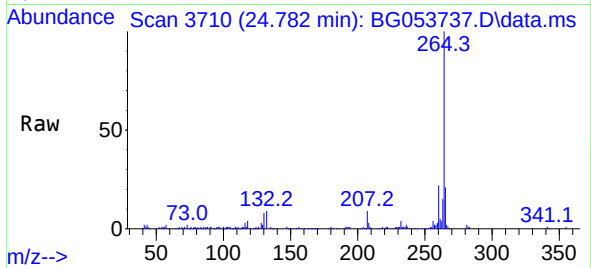

Tgt Ion:264 Resp: 155915

Ion	Ratio	Lower	Upper
264	100		
260	22.1	19.0	28.6
265	21.2	17.4	26.2

