

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053733.D
 Acq On : 27 May 2022 14:52
 Operator : CG/JU
 Sample : N3056-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-12

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	4	9	25	rVB	651042	985460	12.33%	1.972%
2	5.431	407	416	425	rVB	671728	1105317	13.83%	2.212%
3	5.519	425	431	436	rVV	178020	315304	3.95%	0.631%
4	5.590	436	443	455	rVB	66018	181967	2.28%	0.364%
5	5.942	497	503	513	rVB	86995	140369	1.76%	0.281%
6	6.424	576	585	593	rBV	278468	452995	5.67%	0.906%
7	6.923	663	670	677	rBV	269443	437621	5.48%	0.876%
8	7.088	693	698	702	rBV	148433	244504	3.06%	0.489%
9	7.135	702	706	708	rVV	110383	178654	2.24%	0.358%
10	7.170	708	712	722	rVB	177349	291664	3.65%	0.584%
11	7.334	734	740	749	rVB	479918	782724	9.79%	1.566%
12	7.599	778	785	794	rVB	1125463	1841458	23.04%	3.685%
13	7.951	837	845	848	rBV	83628	145872	1.83%	0.292%
14	7.986	848	851	856	rVV	87656	148419	1.86%	0.297%
15	8.069	856	865	872	rVV	579151	1047991	13.11%	2.097%
16	8.133	872	876	884	rVB	71514	115998	1.45%	0.232%
17	8.327	902	909	916	rVB	1407760	2415396	30.22%	4.833%
18	8.444	923	929	933	rBV	173256	273030	3.42%	0.546%
19	8.497	933	938	944	rVB3	66781	119407	1.49%	0.239%
20	8.591	944	954	959	rBV2	180670	331779	4.15%	0.664%
21	8.756	976	982	994	rVB2	44800	90267	1.13%	0.181%
22	8.903	1000	1007	1012	rBV2	129927	241197	3.02%	0.483%
23	8.961	1012	1017	1022	rVB	71411	113799	1.42%	0.228%
24	9.061	1029	1034	1039	rBV	230376	418023	5.23%	0.837%
25	9.144	1039	1048	1057	rVB2	804877	1804735	22.58%	3.611%
26	9.396	1084	1091	1096	rVV	78705	134506	1.68%	0.269%
27	9.584	1118	1123	1128	rBV	134728	219141	2.74%	0.439%
28	9.649	1128	1134	1140	rVB	314535	537502	6.73%	1.076%
29	9.801	1154	1160	1165	rBV	60528	106435	1.33%	0.213%
30	10.007	1189	1195	1205	rVB	526977	899290	11.25%	1.800%
31	10.172	1214	1223	1232	rBV3	761314	2053515	25.69%	4.109%
32	10.266	1232	1239	1243	rBV	778996	1644699	20.58%	3.291%
33	10.395	1255	1261	1267	rVV2	92052	150349	1.88%	0.301%
34	10.465	1267	1273	1282	rVB	182189	318288	3.98%	0.637%
35	10.730	1308	1318	1319	rVV2	66560	121592	1.52%	0.243%
36	10.759	1319	1323	1326	rVV2	119768	238634	2.99%	0.478%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053733.D
 Acq On : 27 May 2022 14:52
 Operator : CG/JU
 Sample : N3056-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-12

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	10.835	1326	1336	1342	rVV	3685608	7991970	100.00%	15.993%
38	11.617	1466	1469	1475	rVV	69190	117525	1.47%	0.235%
39	11.805	1493	1501	1505	rBV	100583	206917	2.59%	0.414%
40	11.863	1505	1511	1515	rVV2	120964	326042	4.08%	0.652%
41	11.910	1515	1519	1521	rVV3	89553	156922	1.96%	0.314%
42	11.952	1521	1526	1537	rVB	179960	418856	5.24%	0.838%
43	12.151	1554	1560	1570	rVB3	67481	123185	1.54%	0.247%
44	12.269	1570	1580	1584	rBV2	77571	181000	2.26%	0.362%
45	12.316	1584	1588	1596	rVB3	101434	219491	2.75%	0.439%
46	12.421	1596	1606	1613	rBV	987927	1669337	20.89%	3.341%
47	12.651	1633	1645	1652	rBV	2512077	4664998	58.37%	9.335%
48	13.215	1734	1741	1747	rVB	802748	1226065	15.34%	2.453%
49	13.426	1768	1777	1784	rBV	475952	754261	9.44%	1.509%
50	13.561	1790	1800	1804	rBV3	68318	131583	1.65%	0.263%
51	13.626	1805	1811	1813	rBV2	100041	162170	2.03%	0.325%
52	13.755	1823	1833	1835	rBV2	168847	309192	3.87%	0.619%
53	13.919	1851	1861	1866	rBV	387510	746231	9.34%	1.493%
54	13.972	1866	1870	1879	rVB2	158398	289759	3.63%	0.580%
55	14.154	1891	1901	1904	rBV	203093	332590	4.16%	0.666%
56	14.184	1904	1906	1918	rVB2	67786	111261	1.39%	0.223%
57	14.319	1918	1929	1940	rVB	164774	294789	3.69%	0.590%
58	14.566	1964	1971	1972	rBV2	66976	100643	1.26%	0.201%
59	14.595	1972	1976	1981	rVV	191180	314193	3.93%	0.629%
60	14.660	1981	1987	1995	rVB	714561	1119068	14.00%	2.239%
61	14.806	2006	2012	2020	rVB	32893	85686	1.07%	0.171%
62	14.994	2037	2044	2050	rVB	64366	113962	1.43%	0.228%
63	15.124	2061	2066	2074	rVV2	33332	81464	1.02%	0.163%
64	15.212	2074	2081	2086	rVV5	64412	129306	1.62%	0.259%
65	15.464	2119	2124	2130	rVB2	107347	166251	2.08%	0.333%
66	15.588	2141	2145	2149	rVV	88165	117926	1.48%	0.236%
67	15.641	2149	2154	2166	rVB	280855	480563	6.01%	0.962%
68	15.852	2185	2190	2195	rBV3	49969	86846	1.09%	0.174%
69	16.052	2219	2224	2225	rBV	83474	98510	1.23%	0.197%
70	16.087	2225	2230	2238	rVB	613319	972831	12.17%	1.947%
71	17.338	2438	2443	2447	rBV	234790	375132	4.69%	0.751%
72	17.385	2447	2451	2457	rVV	548921	787081	9.85%	1.575%
73	17.473	2457	2466	2471	rVB	119639	179787	2.25%	0.360%
74	17.538	2472	2477	2482	rVV3	56365	82239	1.03%	0.165%
75	18.225	2587	2594	2598	rBV2	75267	192859	2.41%	0.386%
76	18.266	2598	2601	2608	rVV	90017	146261	1.83%	0.293%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053733.D
 Acq On : 27 May 2022 14:52
 Operator : CG/JU
 Sample : N3056-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-12

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	18.413	2618	2626	2630	rVV4	73873	177682	2.22%	0.356%
78	19.036	2726	2732	2739	rVB2	64444	111815	1.40%	0.224%
79	19.394	2787	2793	2799	rBV	66846	103388	1.29%	0.207%
80	19.759	2846	2855	2863	rBV	113521	189362	2.37%	0.379%
81	19.952	2882	2888	2895	rVB	1238696	1646198	20.60%	3.294%
82	20.499	2977	2981	2986	rBV	49898	90872	1.14%	0.182%
83	21.239	3102	3107	3119	rVB2	72626	137098	1.72%	0.274%
84	21.597	3162	3168	3174	rBV	242224	412370	5.16%	0.825%
85	24.781	3700	3710	3720	rBV	142426	390821	4.89%	0.782%




Sum of corrected areas: 49972259

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053733.D
Acq On : 27 May 2022 14:52
Operator : CG/JU
Sample : N3056-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

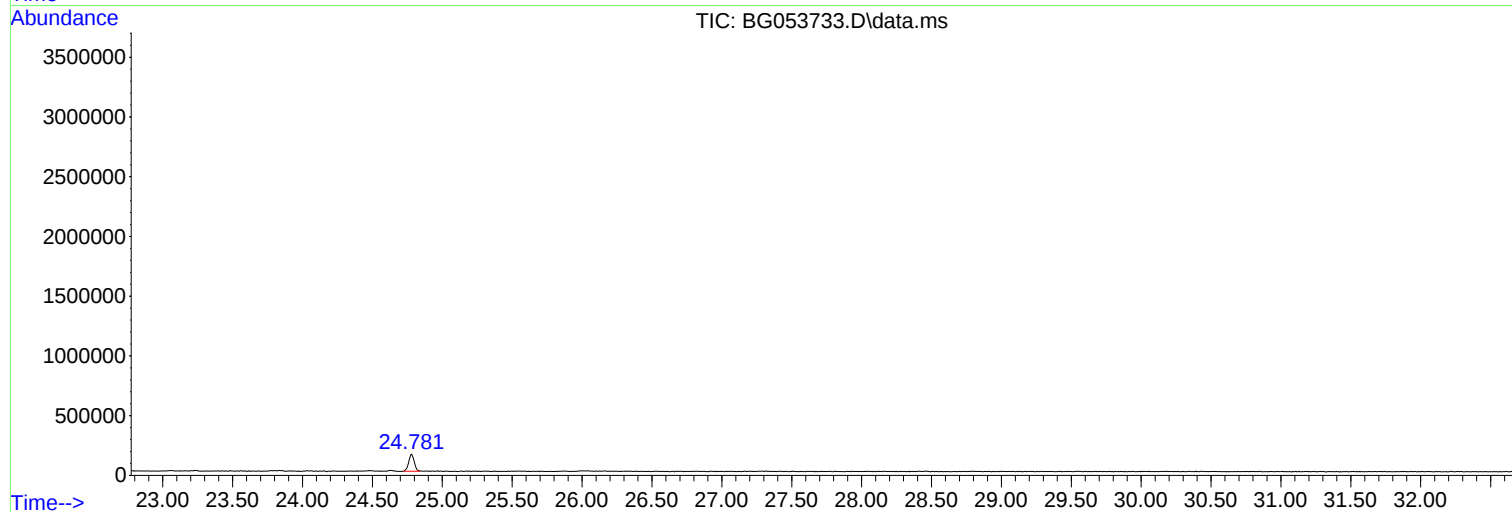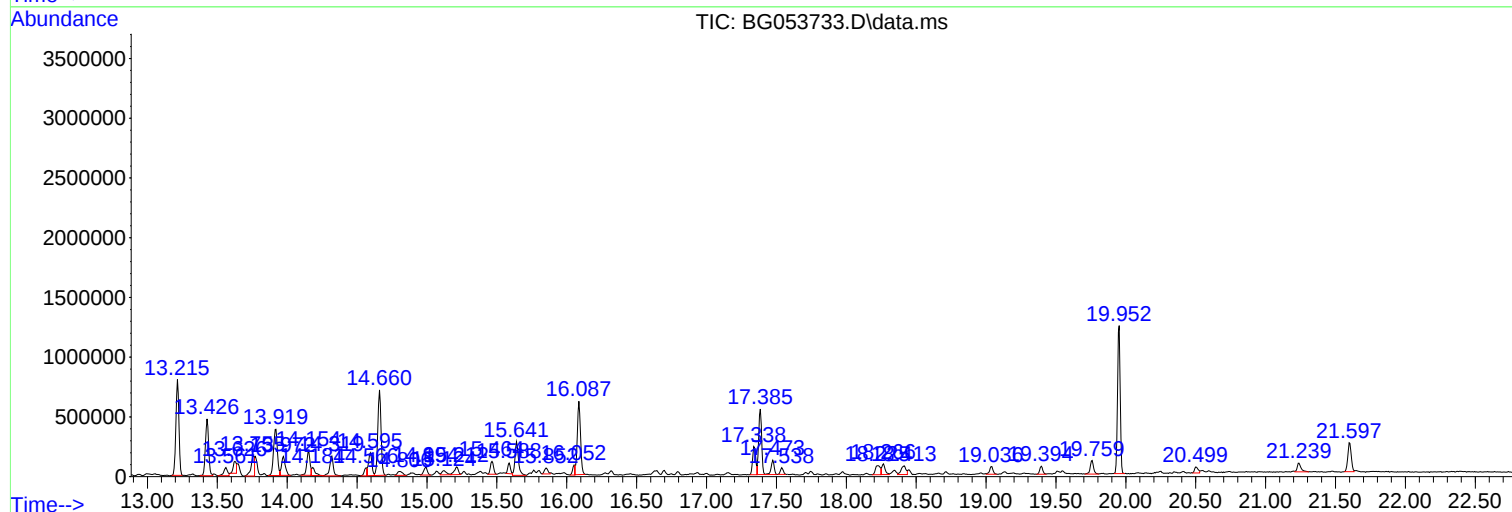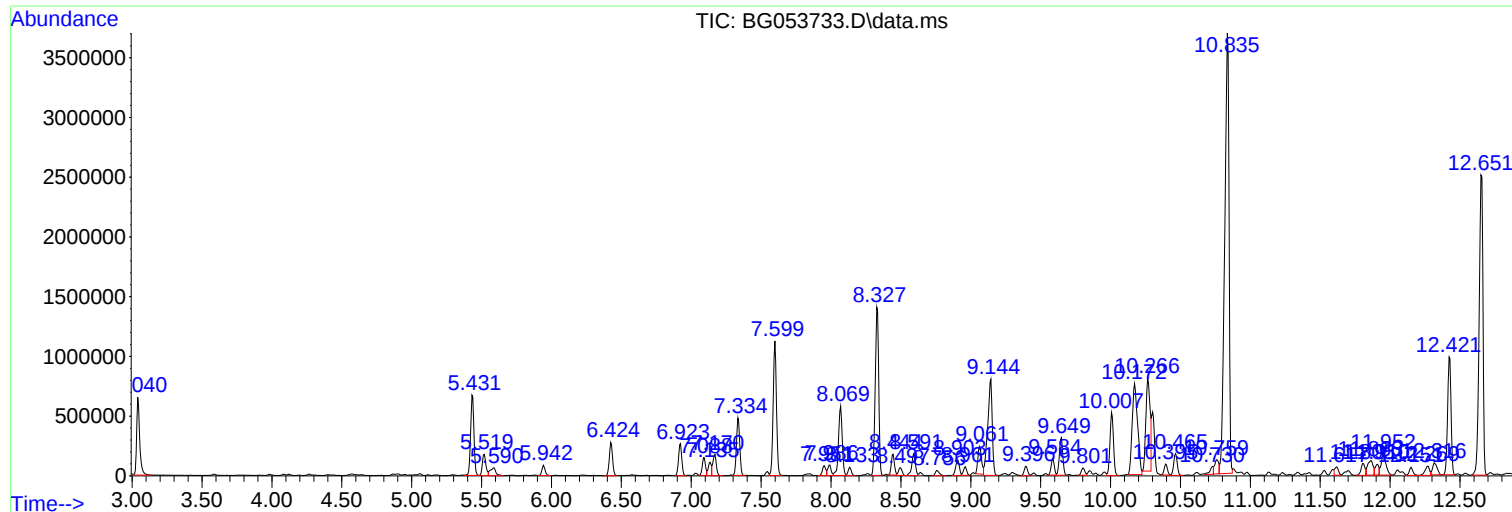

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053733.D
Acq On : 27 May 2022 14:52
Operator : CG/JU
Sample : N3056-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053733.D
Acq On : 27 May 2022 14:52
Operator : CG/JU
Sample : N3056-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc