

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053736.D
 Acq On : 27 May 2022 16:51
 Operator : CG/JU
 Sample : N3072-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RT-4206

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.041	4	9	24	rVB	196202	295535	29.22%	4.992%
2	5.027	341	347	354	rVB3	6749	12910	1.28%	0.218%
3	5.514	423	430	446	rBV	255759	436151	43.12%	7.368%
4	7.130	699	705	718	rBV	286672	504794	49.90%	8.527%
5	7.946	838	844	858	rBV	78195	132529	13.10%	2.239%
6	9.115	1036	1043	1056	rBV	173245	321292	31.76%	5.427%
7	10.760	1316	1323	1336	rBV	102068	187273	18.51%	3.163%
8	13.215	1734	1741	1749	rBV	418846	644857	63.75%	10.893%
9	14.596	1968	1976	1983	rBV	187393	293211	28.99%	4.953%
10	16.088	2224	2230	2244	rBV	386086	644441	63.71%	10.886%
11	17.339	2437	2443	2449	rBV	265564	390243	38.58%	6.592%
12	19.395	2788	2793	2801	rBV	33212	51647	5.11%	0.872%
13	19.759	2851	2855	2861	rVB	31554	44280	4.38%	0.748%
14	19.947	2882	2887	2893	rBV	774868	1011559	100.00%	17.088%
15	20.247	2932	2938	2943	rVB7	8608	13266	1.31%	0.224%
16	21.234	3101	3106	3113	rBV3	31135	58870	5.82%	0.994%
17	21.604	3161	3169	3174	rBV	261670	446394	44.13%	7.541%
18	23.772	3533	3538	3542	rBV3	13291	27717	2.74%	0.468%
19	24.776	3701	3709	3722	rVB2	140481	402898	39.83%	6.806%




Sum of corrected areas: 5919867

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053736.D
Acq On : 27 May 2022 16:51
Operator : CG/JU
Sample : N3072-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RT-4206

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

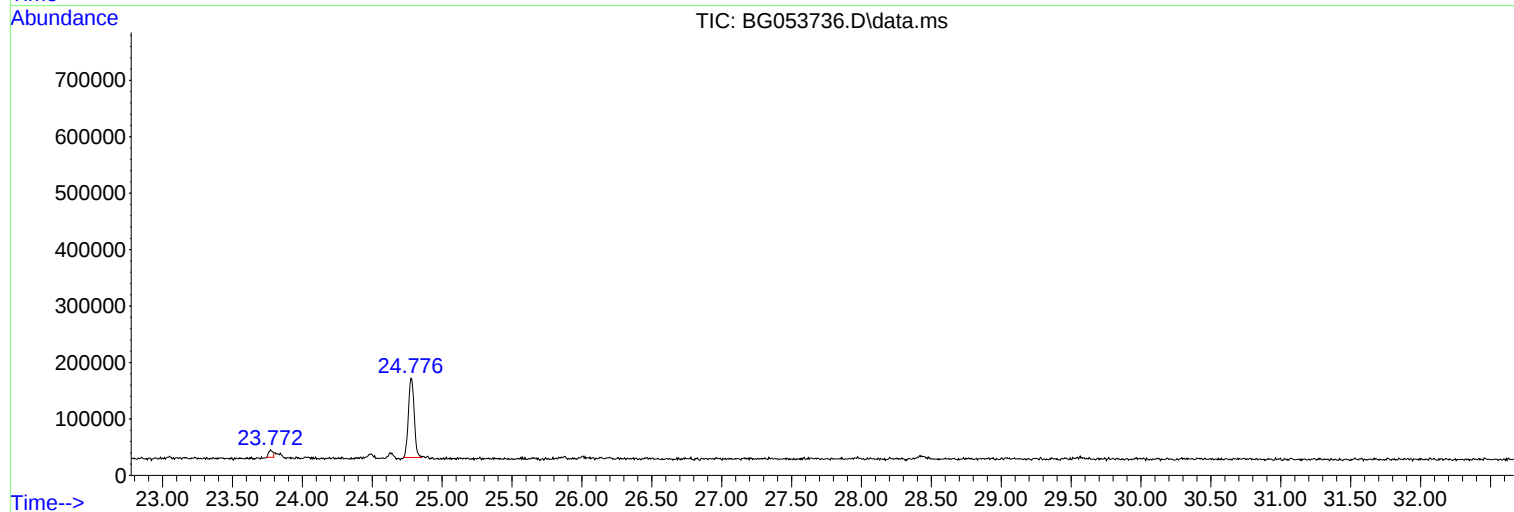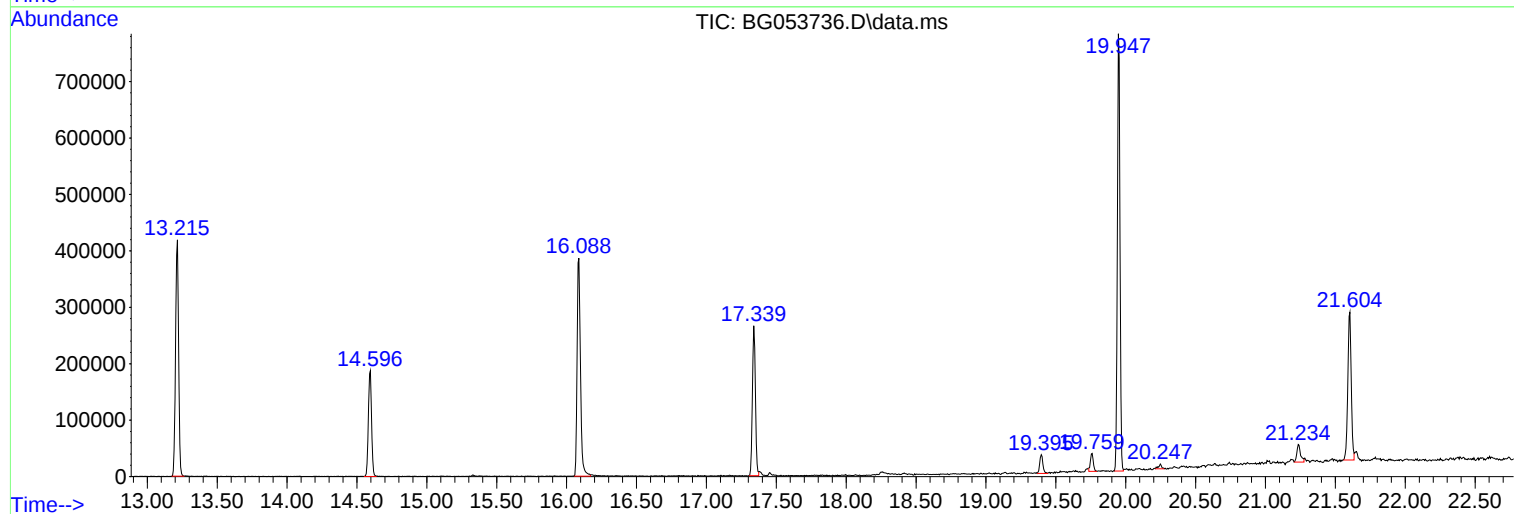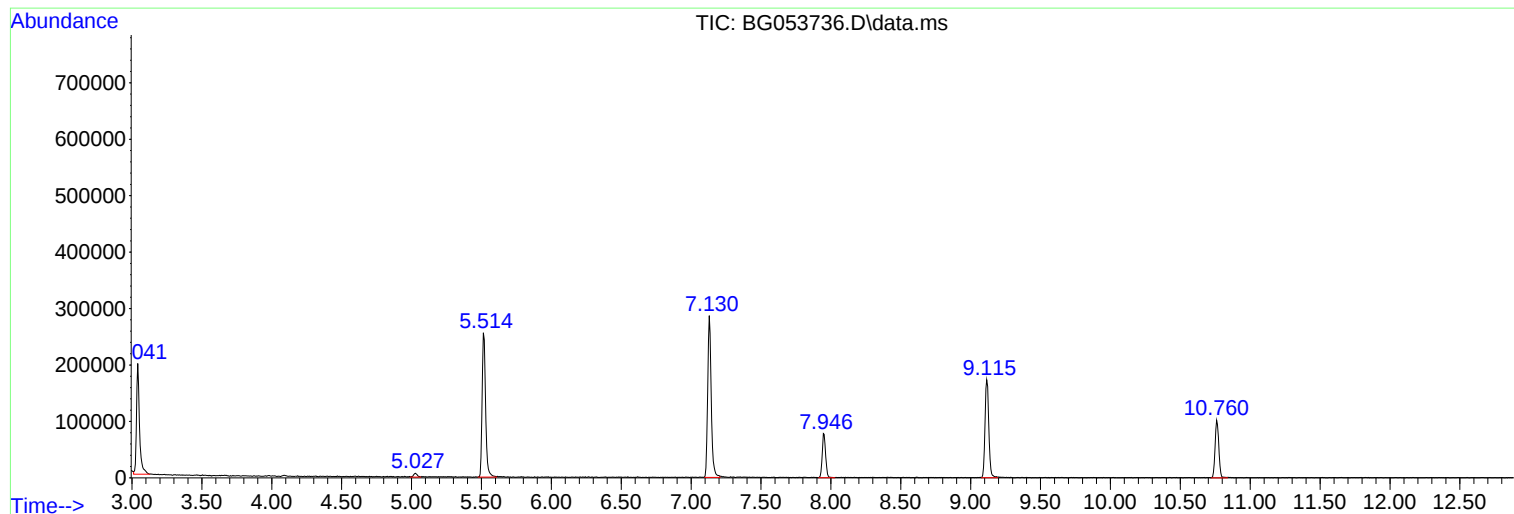

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053736.D
Acq On : 27 May 2022 16:51
Operator : CG/JU
Sample : N3072-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RT-4206

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053736.D
Acq On : 27 May 2022 16:51
Operator : CG/JU
Sample : N3072-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RT-4206

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------