

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053737.D
 Acq On : 27 May 2022 17:31
 Operator : CG/JU
 Sample : N3072-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PSC-124030

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053737.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	4	9	25	rVB	234501	371242	27.22%	5.221%
2	5.026	342	347	356	rVB3	10173	18223	1.34%	0.256%
3	5.519	424	431	444	rBV	319761	554890	40.68%	7.804%
4	7.129	698	705	722	rBV	359160	640889	46.99%	9.013%
5	7.951	839	845	853	rVB	78291	127294	9.33%	1.790%
6	9.115	1036	1043	1056	rBV	226072	410023	30.06%	5.766%
7	10.759	1316	1323	1331	rBV	98857	180910	13.26%	2.544%
8	13.215	1731	1741	1749	rBV	529990	820108	60.13%	11.534%
9	14.590	1969	1975	1984	rBV	175017	279349	20.48%	3.929%
10	16.087	2223	2230	2245	rBV	540797	844562	61.92%	11.878%
11	17.339	2435	2443	2449	rBV	245766	382210	28.02%	5.375%
12	17.380	2449	2450	2458	rVB3	11398	13922	1.02%	0.196%
13	18.238	2588	2596	2607	rBV8	11861	40085	2.94%	0.564%
14	19.395	2788	2793	2800	rBV2	35973	50851	3.73%	0.715%
15	19.759	2851	2855	2860	rVB	26470	41807	3.07%	0.588%
16	19.953	2881	2888	2894	rBV	1013149	1363887	100.00%	19.181%
17	20.247	2935	2938	2943	rVB5	10504	13715	1.01%	0.193%
18	21.233	3102	3106	3119	rVB4	56164	95208	6.98%	1.339%
19	21.604	3160	3169	3174	rBV2	260374	449252	32.94%	6.318%
20	23.789	3535	3541	3544	rBV6	6526	14623	1.07%	0.206%
21	24.782	3701	3710	3722	rVB2	147479	397525	29.15%	5.591%




Sum of corrected areas: 7110575

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053737.D
Acq On : 27 May 2022 17:31
Operator : CG/JU
Sample : N3072-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PSC-124030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

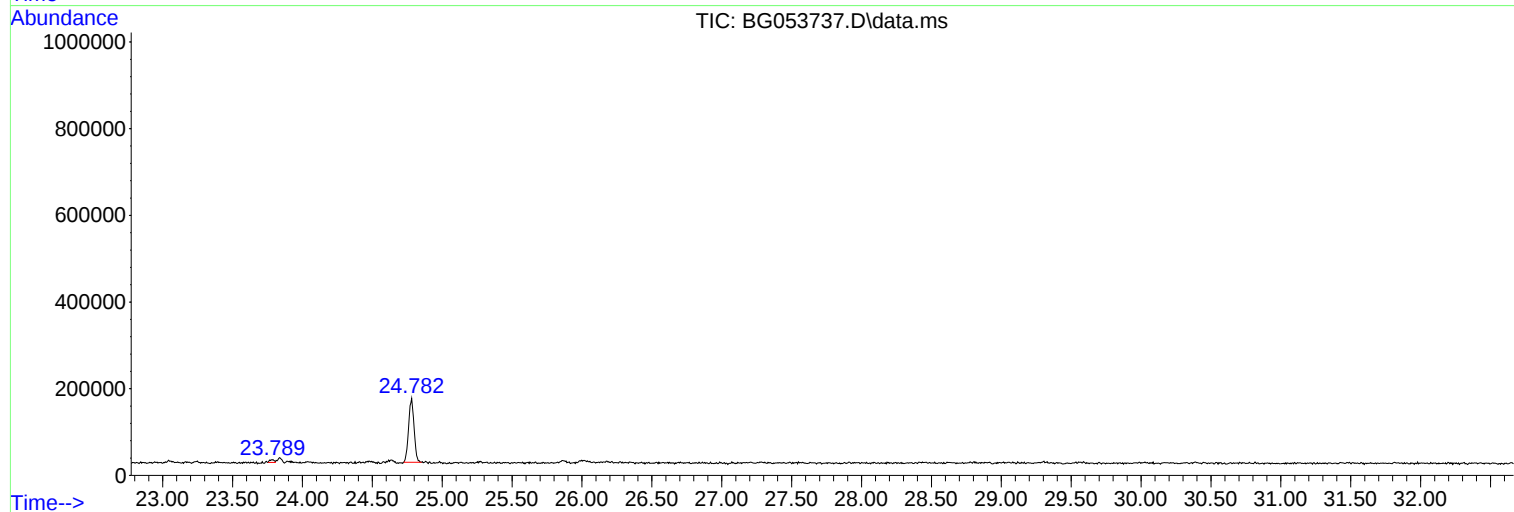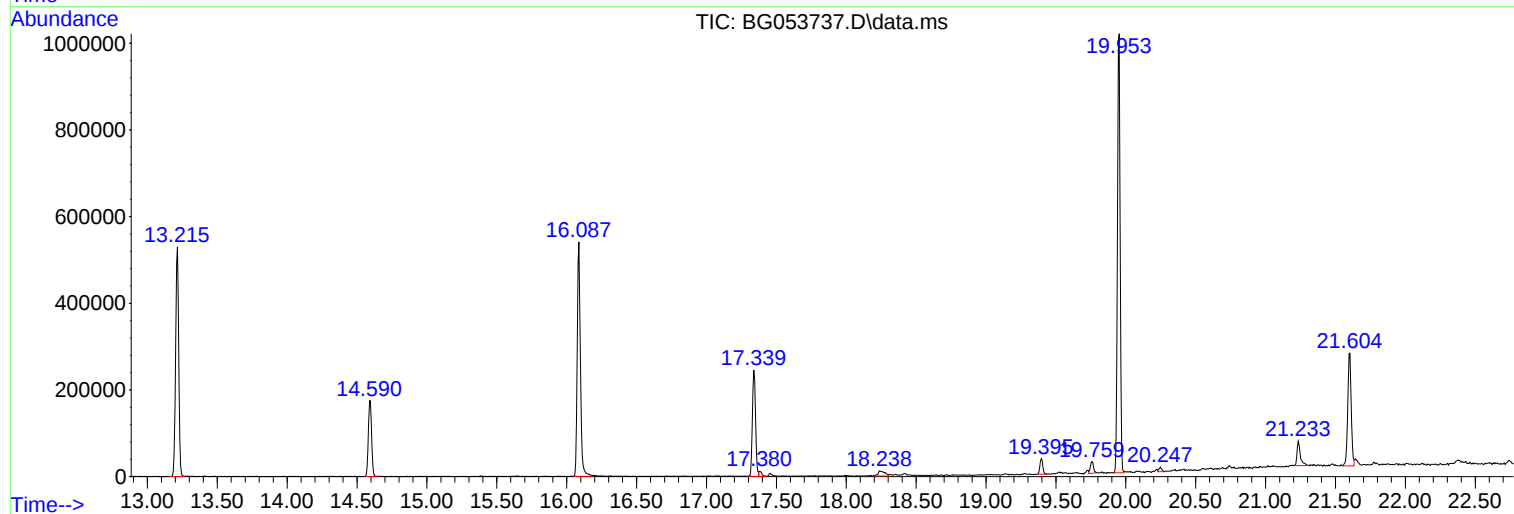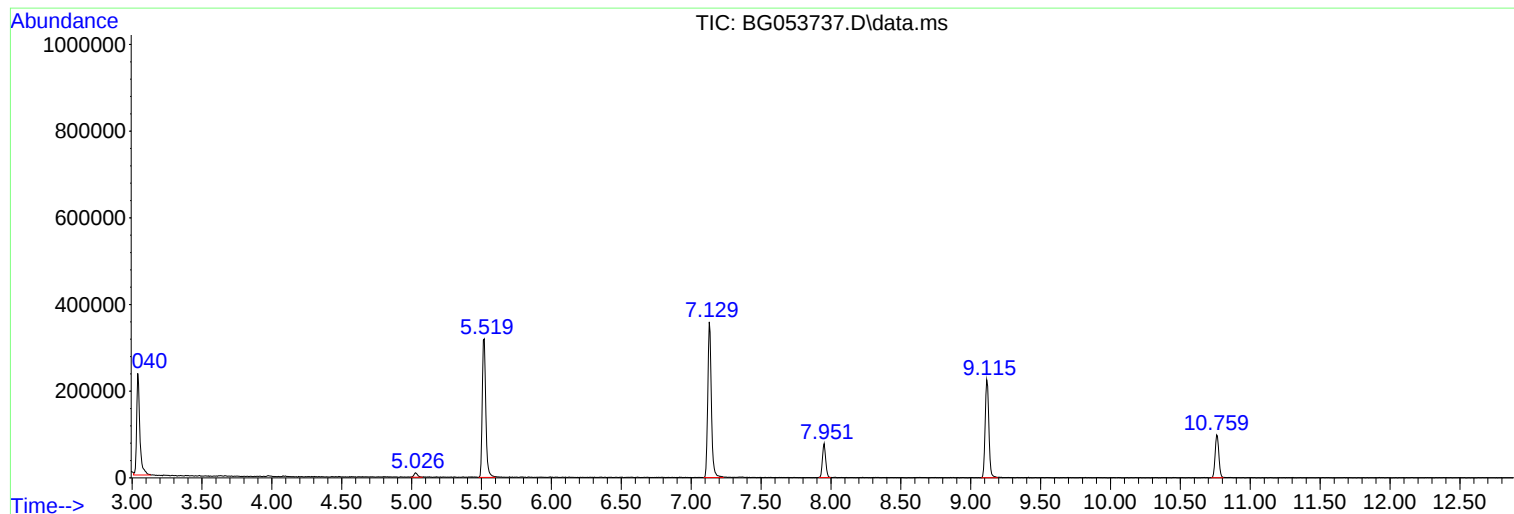

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053737.D
Acq On : 27 May 2022 17:31
Operator : CG/JU
Sample : N3072-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PSC-124030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053737.D
Acq On : 27 May 2022 17:31
Operator : CG/JU
Sample : N3072-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PSC-124030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------