

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053738.D
 Acq On : 27 May 2022 18:12
 Operator : CG/JU
 Sample : N3067-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 33686

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.521	425	431	445	rBV	327192	595367	4.46%	0.204%
2	7.142	696	707	722	rBV	323359	707726	5.30%	0.242%
3	7.958	822	846	847	rBV2	896429	3620566	27.12%	1.238%
4	8.264	877	898	902	rBV	741105	2977028	22.30%	1.018%
5	8.334	902	910	929	rVB	1012745	2729710	20.45%	0.933%
6	8.740	968	979	999	rBV	298320	685370	5.13%	0.234%
7	9.674	1132	1138	1151	rVB	450956	824386	6.17%	0.282%
8	11.789	1491	1498	1511	rVB	343053	565074	4.23%	0.193%
9	12.388	1594	1600	1613	rVV2	321677	691192	5.18%	0.236%
10	12.605	1632	1637	1645	rVV2	357952	626384	4.69%	0.214%
11	12.817	1666	1673	1681	rBV	447353	742528	5.56%	0.254%
12	12.958	1689	1697	1702	rVV4	366469	987190	7.39%	0.338%
13	13.010	1702	1706	1717	rVV	703460	1217173	9.12%	0.416%
14	13.104	1717	1722	1733	rVV	655649	1043736	7.82%	0.357%
15	13.222	1733	1742	1756	rVB2	1196009	2077756	15.56%	0.711%
16	13.563	1793	1800	1817	rVB	1324215	2058211	15.42%	0.704%
17	14.643	1979	1984	1990	rVV	1910378	2843215	21.30%	0.972%
18	15.137	2048	2068	2074	rBV2	1626316	6518805	48.83%	2.229%
19	15.354	2099	2105	2112	rVV	600327	949891	7.11%	0.325%
20	15.601	2141	2147	2152	rVV	1785133	2873154	21.52%	0.983%
21	15.654	2152	2156	2162	rVV	1040254	1446693	10.84%	0.495%
22	15.818	2177	2184	2196	rVB	1708101	3065558	22.96%	1.048%
23	15.983	2207	2212	2222	rVB	1157059	1629212	12.20%	0.557%
24	16.100	2224	2232	2233	rBV2	420554	625848	4.69%	0.214%
25	16.124	2233	2236	2248	rVB2	599731	924938	6.93%	0.316%
26	16.230	2248	2254	2262	rBV	1824023	2626401	19.67%	0.898%
27	16.494	2288	2299	2308	rVB	475270	1033826	7.74%	0.354%
28	16.817	2339	2354	2364	rBV	1850319	4671644	34.99%	1.598%
29	17.052	2386	2394	2399	rVV2	2859051	4626879	34.65%	1.582%
30	17.275	2425	2432	2438	rVB	661792	1056179	7.91%	0.361%
31	17.346	2438	2444	2450	rBV3	905620	1614132	12.09%	0.552%
32	17.557	2476	2480	2482	rVV	639913	921437	6.90%	0.315%
33	17.587	2482	2485	2493	rVB	1172449	1632372	12.23%	0.558%
34	17.669	2494	2499	2503	rBV	554578	831805	6.23%	0.284%
35	17.716	2503	2507	2517	rVB	818506	1258788	9.43%	0.430%
36	17.816	2517	2524	2538	rBV2	3069937	7398687	55.42%	2.530%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053738.D
 Acq On : 27 May 2022 18:12
 Operator : CG/JU
 Sample : N3067-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 33686

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.974	2545	2551	2554	rBV	1928174	3020810	22.63%	1.033%
38	18.010	2554	2557	2567	rVB	1125896	1852330	13.87%	0.633%
39	18.121	2570	2576	2578	rBV	1833304	2691357	20.16%	0.920%
40	18.162	2578	2583	2592	rVB	1561785	3243565	24.29%	1.109%
41	18.315	2599	2609	2615	rBV3	5195760	11701358	87.64%	4.002%
42	18.515	2639	2643	2648	rBV	798263	1051554	7.88%	0.360%
43	18.632	2657	2663	2671	rVB6	521647	1265894	9.48%	0.433%
44	18.814	2689	2694	2699	rBV3	342635	653381	4.89%	0.223%
45	18.991	2717	2724	2735	rVB2	4140554	7581427	56.78%	2.593%
46	19.102	2736	2743	2748	rBV	6001626	9135821	68.43%	3.124%
47	19.149	2748	2751	2757	rVV	611532	901166	6.75%	0.308%
48	19.208	2757	2761	2767	rVV2	636381	992271	7.43%	0.339%
49	19.408	2789	2795	2796	rBV	1380815	2012128	15.07%	0.688%
50	19.437	2796	2800	2804	rVB	1517403	2424519	18.16%	0.829%
51	19.554	2812	2820	2822	rBV	2150616	3248592	24.33%	1.111%
52	19.596	2822	2827	2838	rVB	4182259	8554091	64.07%	2.925%
53	19.719	2844	2848	2851	rVV	1961450	2769326	20.74%	0.947%
54	19.760	2851	2855	2862	rVB2	1804032	2775598	20.79%	0.949%
55	19.842	2863	2869	2877	rBV3	3203146	6183292	46.31%	2.115%
56	19.989	2884	2894	2901	rBV2	3598495	6768362	50.69%	2.315%
57	20.118	2911	2916	2927	rVB	1032057	1853776	13.88%	0.634%
58	20.230	2931	2935	2938	rBV2	568741	793466	5.94%	0.271%
59	20.295	2942	2946	2950	rBV2	374856	606852	4.55%	0.208%
60	20.342	2950	2954	2958	rBV3	280975	566538	4.24%	0.194%
61	20.400	2959	2964	2968	rVB2	4149727	5153342	38.60%	1.762%
62	20.512	2976	2983	2987	rVB	4937836	7037553	52.71%	2.407%
63	20.618	2995	3001	3004	rBV2	944461	1485685	11.13%	0.508%
64	20.647	3004	3006	3011	rVB3	510588	597248	4.47%	0.204%
65	20.841	3035	3039	3044	rBV	915062	1184444	8.87%	0.405%
66	20.911	3044	3051	3056	rVB2	2219480	3268727	24.48%	1.118%
67	21.011	3060	3068	3073	rBV	4409439	8932983	66.91%	3.055%
68	21.052	3073	3075	3079	rVB3	529685	582077	4.36%	0.199%
69	21.117	3080	3086	3091	rBV	2059108	3377764	25.30%	1.155%
70	21.170	3091	3095	3101	rVB	1382997	2120907	15.89%	0.725%
71	21.235	3101	3106	3123	rVB2	2311658	4810789	36.03%	1.645%
72	21.381	3123	3131	3138	rBV	3371880	5949121	44.56%	2.034%
73	21.458	3138	3144	3147	rBV	1937545	2494506	18.68%	0.853%
74	21.493	3147	3150	3154	rBV	575838	670413	5.02%	0.229%
75	21.616	3165	3171	3174	rBV3	448448	916459	6.86%	0.313%
76	21.658	3175	3178	3181	rVV2	463680	783519	5.87%	0.268%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053738.D
 Acq On : 27 May 2022 18:12
 Operator : CG/JU
 Sample : N3067-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 33686

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	21.699	3182	3185	3193	rVB3	481666	1072910	8.04%	0.367%
78	21.939	3216	3226	3235	rBV	4323864	7994770	59.88%	2.734%
79	22.057	3240	3246	3250	rBV	455330	891846	6.68%	0.305%
80	22.239	3273	3277	3281	rBV	416671	614071	4.60%	0.210%
81	22.345	3289	3295	3298	rBV	554896	1069768	8.01%	0.366%
82	22.380	3298	3301	3314	rVB5	556312	1412449	10.58%	0.483%
83	22.568	3323	3333	3341	rBV	3232252	8947484	67.02%	3.060%
84	22.639	3342	3345	3350	rVV3	324784	578295	4.33%	0.198%
85	22.715	3352	3358	3363	rVB2	1212073	2462049	18.44%	0.842%
86	22.768	3363	3367	3369	rBV	486085	738337	5.53%	0.252%
87	22.803	3370	3373	3378	rVB2	791025	1174324	8.80%	0.402%
88	22.879	3379	3386	3391	rBV2	1528733	3126370	23.42%	1.069%
89	23.067	3409	3418	3434	rVB2	2697983	7301300	54.69%	2.497%
90	23.202	3436	3441	3446	rBV4	410539	951464	7.13%	0.325%
91	23.614	3506	3511	3526	rVB3	403015	1249143	9.36%	0.427%
92	23.849	3538	3551	3567	rVB2	2441810	7199583	53.92%	2.462%
93	24.777	3694	3709	3723	rBV2	1794111	7402548	55.44%	2.531%
94	24.988	3736	3745	3753	rBV	692404	1894638	14.19%	0.648%
95	25.141	3765	3771	3779	rVB2	358039	931015	6.97%	0.318%
96	25.241	3779	3788	3808	rVB2	751813	2536077	18.99%	0.867%
97	25.535	3824	3838	3851	rBV2	1155799	4381788	32.82%	1.498%
98	26.862	4033	4064	4073	rVB3	2547936	13351360	100.00%	4.566%
99	28.278	4286	4305	4329	rVB4	856728	5355418	40.11%	1.831%
100	30.146	4602	4623	4642	rVB4	1187490	7072878	52.97%	2.419%




Sum of corrected areas: 292421757

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053738.D
Acq On : 27 May 2022 18:12
Operator : CG/JU
Sample : N3067-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
33686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

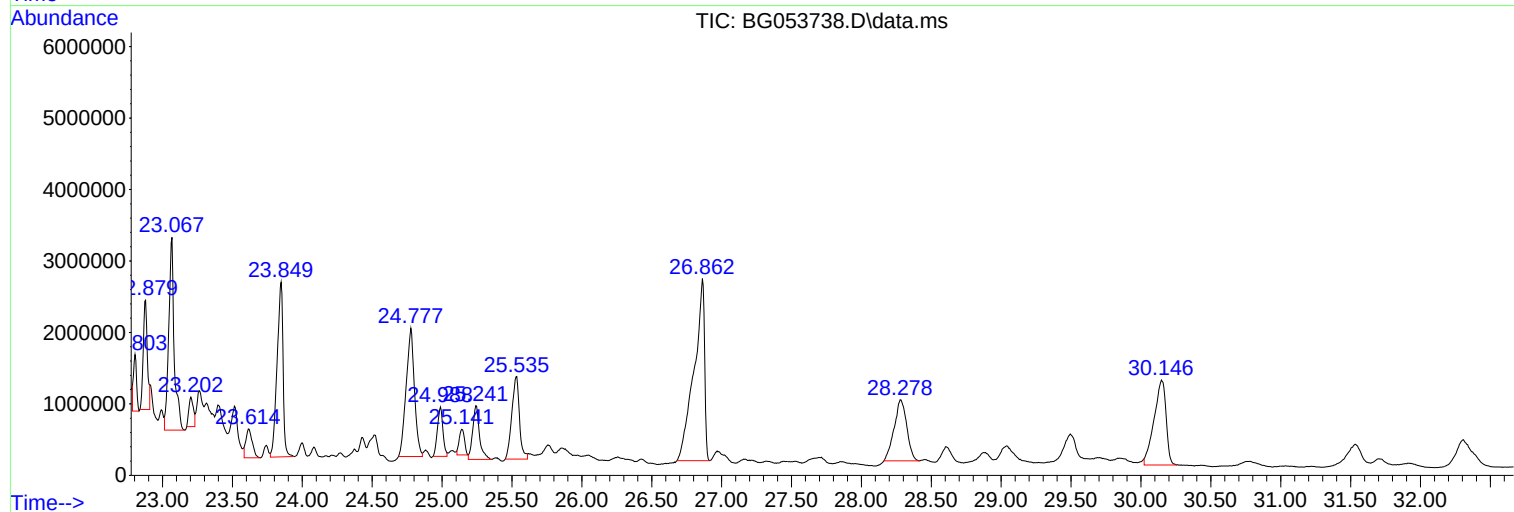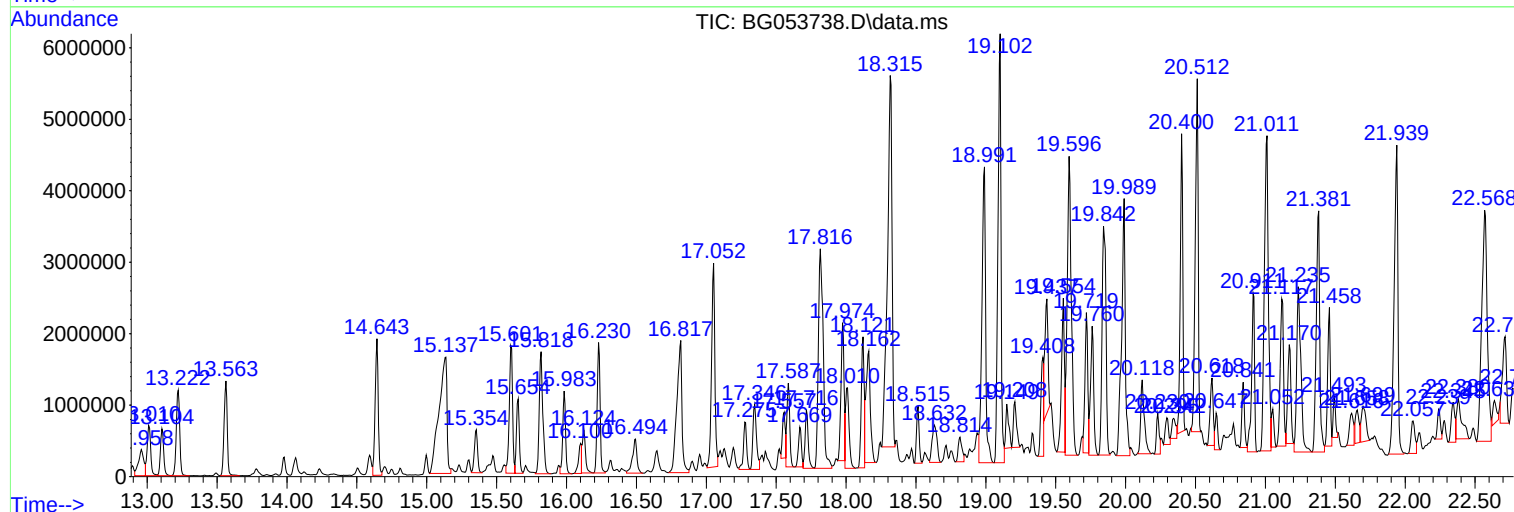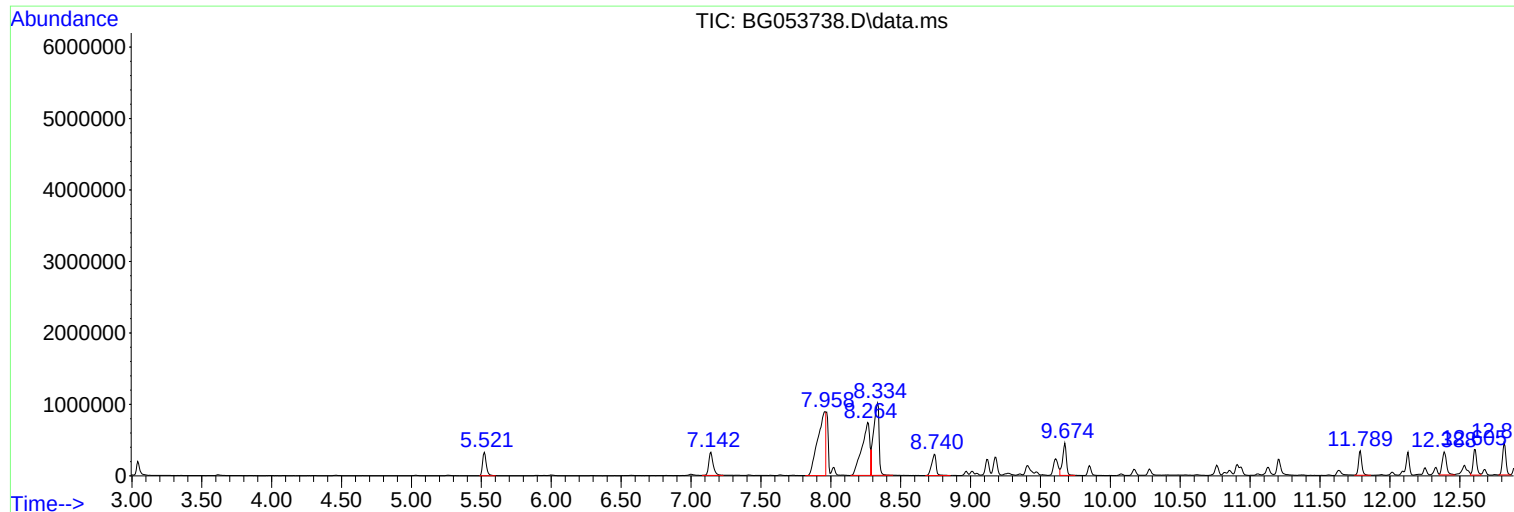

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053738.D
Acq On : 27 May 2022 18:12
Operator : CG/JU
Sample : N3067-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
33686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053738.D
Acq On : 27 May 2022 18:12
Operator : CG/JU
Sample : N3067-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
33686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------