

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053740.D
 Acq On : 27 May 2022 19:32
 Operator : CG/JU
 Sample : N3072-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PSC-124035

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.044	4	9	24	rVB	183457	293193	5.31%	0.526%
2	5.534	427	433	445	rBV	315619	528020	9.55%	0.948%
3	7.162	703	710	720	rBV	356013	636675	11.52%	1.143%
4	7.949	838	844	853	rVB	90540	150928	2.73%	0.271%
5	9.118	1036	1043	1053	rBV	226598	402313	7.28%	0.722%
6	10.763	1315	1323	1327	rBV	130732	229931	4.16%	0.413%
7	10.815	1327	1332	1339	rVB	219313	385820	6.98%	0.692%
8	12.425	1599	1606	1614	rBV	167147	274600	4.97%	0.493%
9	12.636	1632	1642	1653	rVB	119774	211327	3.82%	0.379%
10	13.218	1734	1741	1749	rVB	469403	729300	13.20%	1.309%
11	13.424	1769	1776	1784	rVB	50309	89218	1.61%	0.160%
12	13.764	1824	1834	1843	rBV3	60691	165276	2.99%	0.297%
13	13.917	1852	1860	1865	rBV	115270	212921	3.85%	0.382%
14	13.970	1865	1869	1876	rVB	79711	126591	2.29%	0.227%
15	14.322	1918	1929	1938	rBV	93575	167055	3.02%	0.300%
16	14.599	1965	1976	1981	rBV2	213209	395592	7.16%	0.710%
17	14.663	1981	1987	1993	rVB	487439	792637	14.34%	1.422%
18	14.992	2037	2043	2050	rVV	466949	746065	13.50%	1.339%
19	15.209	2072	2080	2085	rBV3	51530	95840	1.73%	0.172%
20	15.386	2102	2110	2113	rBV4	39536	90672	1.64%	0.163%
21	15.644	2147	2154	2163	rVB	563541	890344	16.11%	1.598%
22	15.768	2172	2175	2178	rVV	77010	110771	2.00%	0.199%
23	15.809	2178	2182	2186	rVV	89562	138476	2.51%	0.248%
24	15.938	2199	2204	2211	rVB	198380	319476	5.78%	0.573%
25	16.091	2219	2230	2238	rBV2	650435	1186779	21.48%	2.130%
26	16.179	2238	2245	2250	rVB2	52183	110527	2.00%	0.198%
27	16.320	2266	2269	2279	rVB2	54155	89585	1.62%	0.161%
28	16.649	2312	2325	2330	rBV3	119284	325589	5.89%	0.584%
29	16.878	2355	2364	2367	rBV3	111677	231696	4.19%	0.416%
30	16.913	2367	2370	2374	rVV2	104025	174828	3.16%	0.314%
31	17.001	2378	2385	2392	rVV	300080	517454	9.36%	0.929%
32	17.078	2392	2398	2405	rVV3	121001	289974	5.25%	0.520%
33	17.160	2405	2412	2422	rVB	238176	409085	7.40%	0.734%
34	17.348	2439	2444	2446	rBV	241186	358224	6.48%	0.643%
35	17.401	2446	2453	2458	rVV	3312508	5526328	100.00%	9.917%
36	17.483	2458	2467	2472	rVV	890747	1398016	25.30%	2.509%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053740.D
 Acq On : 27 May 2022 19:32
 Operator : CG/JU
 Sample : N3072-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PSC-124035

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.536	2472	2476	2481	rVB3	69035	124005	2.24%	0.223%
38	17.753	2502	2513	2527	rBV2	279134	731553	13.24%	1.313%
39	17.859	2527	2531	2538	rVB3	74080	115972	2.10%	0.208%
40	17.929	2538	2543	2551	rVB4	96981	182115	3.30%	0.327%
41	18.223	2584	2593	2597	rBV	491476	837211	15.15%	1.502%
42	18.270	2597	2601	2607	rVB	684668	1029616	18.63%	1.848%
43	18.352	2607	2615	2620	rBV	287345	438730	7.94%	0.787%
44	18.423	2620	2627	2630	rBV2	597243	1116529	20.20%	2.004%
45	18.452	2630	2632	2639	rVB	298416	384685	6.96%	0.690%
46	18.523	2640	2644	2648	rBV3	71851	97641	1.77%	0.175%
47	18.570	2648	2652	2656	rVV2	63849	80677	1.46%	0.145%
48	18.716	2672	2677	2681	rVV	326754	460413	8.33%	0.826%
49	18.769	2681	2686	2691	rVV	242429	343798	6.22%	0.617%
50	18.963	2715	2719	2724	rVB3	97239	141858	2.57%	0.255%
51	19.010	2724	2727	2731	rBV	88610	108487	1.96%	0.195%
52	19.051	2731	2734	2739	rVB	101469	131663	2.38%	0.236%
53	19.134	2742	2748	2752	rBV2	214216	382809	6.93%	0.687%
54	19.286	2768	2774	2781	rVB2	226995	444201	8.04%	0.797%
55	19.410	2787	2795	2800	rBV	2948793	4828141	87.37%	8.664%
56	19.463	2800	2804	2807	rVV2	74377	103916	1.88%	0.186%
57	19.498	2807	2810	2815	rVB2	100659	145718	2.64%	0.261%
58	19.603	2823	2828	2830	rBV3	65742	98621	1.78%	0.177%
59	19.645	2831	2835	2838	rVB	88895	120436	2.18%	0.216%
60	19.739	2845	2851	2852	rBV	712040	996806	18.04%	1.789%
61	19.774	2852	2857	2863	rVV	2310505	3608381	65.29%	6.475%
62	19.833	2863	2867	2873	rVB2	228713	361564	6.54%	0.649%
63	19.950	2874	2887	2892	rBV2	735207	1319188	23.87%	2.367%
64	20.009	2892	2897	2902	rVB	144083	247021	4.47%	0.443%
65	20.085	2903	2910	2917	rBV3	241108	657082	11.89%	1.179%
66	20.144	2917	2920	2927	rVB	51878	91613	1.66%	0.164%
67	20.220	2927	2933	2935	rBV3	186785	352722	6.38%	0.633%
68	20.256	2935	2939	2944	rVB	327619	492680	8.92%	0.884%
69	20.350	2951	2955	2959	rBV	145823	210654	3.81%	0.378%
70	20.414	2959	2966	2970	rVV2	311521	621698	11.25%	1.116%
71	20.449	2970	2972	2975	rVV	80622	83783	1.52%	0.150%
72	20.491	2975	2979	2984	rVB	89513	131747	2.38%	0.236%
73	20.555	2985	2990	2993	rBV	148215	216843	3.92%	0.389%
74	20.596	2993	2997	3001	rVB3	152957	211939	3.84%	0.380%
75	20.802	3029	3032	3035	rBV3	51722	79527	1.44%	0.143%
76	21.013	3063	3068	3073	rBV	378990	509699	9.22%	0.915%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053740.D
 Acq On : 27 May 2022 19:32
 Operator : CG/JU
 Sample : N3072-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PSC-124035

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	21.190	3092	3098	3102	rBV2	211507	428166	7.75%	0.768%
78	21.237	3102	3106	3110	rVV2	307766	495633	8.97%	0.889%
79	21.289	3110	3115	3120	rVV3	211039	415485	7.52%	0.746%
80	21.348	3120	3125	3131	rVB	308450	503633	9.11%	0.904%
81	21.595	3156	3167	3173	rBV3	1301721	2794257	50.56%	5.014%
82	21.660	3173	3178	3190	rVB	1046604	1847709	33.43%	3.316%
83	21.806	3199	3203	3211	rVB	94066	161768	2.93%	0.290%
84	21.883	3212	3216	3219	rBV5	48048	92595	1.68%	0.166%
85	22.018	3233	3239	3245	rBV2	139766	284797	5.15%	0.511%
86	22.077	3245	3249	3254	rVV7	46210	82398	1.49%	0.148%
87	22.253	3275	3279	3284	rBV4	61355	102748	1.86%	0.184%
88	22.329	3287	3292	3297	rVV	233447	443714	8.03%	0.796%
89	22.400	3300	3304	3311	rVB	121434	229065	4.14%	0.411%
90	22.599	3334	3338	3343	rBV2	81906	161633	2.92%	0.290%
91	22.735	3358	3361	3368	rVB4	75098	139328	2.52%	0.250%
92	23.005	3402	3407	3413	rBV4	44742	104033	1.88%	0.187%
93	23.798	3532	3542	3548	rBV	549991	1749593	31.66%	3.140%
94	24.039	3577	3583	3590	rVB	109813	245523	4.44%	0.441%
95	24.503	3655	3662	3675	rVB	272385	846035	15.31%	1.518%
96	24.655	3678	3688	3699	rVB	445152	1209175	21.88%	2.170%
97	24.796	3704	3712	3718	rVV	143748	398620	7.21%	0.715%
98	24.879	3720	3726	3740	rVB3	108548	386528	6.99%	0.694%
99	28.450	4324	4334	4351	rVB3	167094	754894	13.66%	1.355%
100	29.578	4516	4526	4541	rVB	92754	404806	7.33%	0.726%




Sum of corrected areas: 55725004

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053740.D
Acq On : 27 May 2022 19:32
Operator : CG/JU
Sample : N3072-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PSC-124035

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

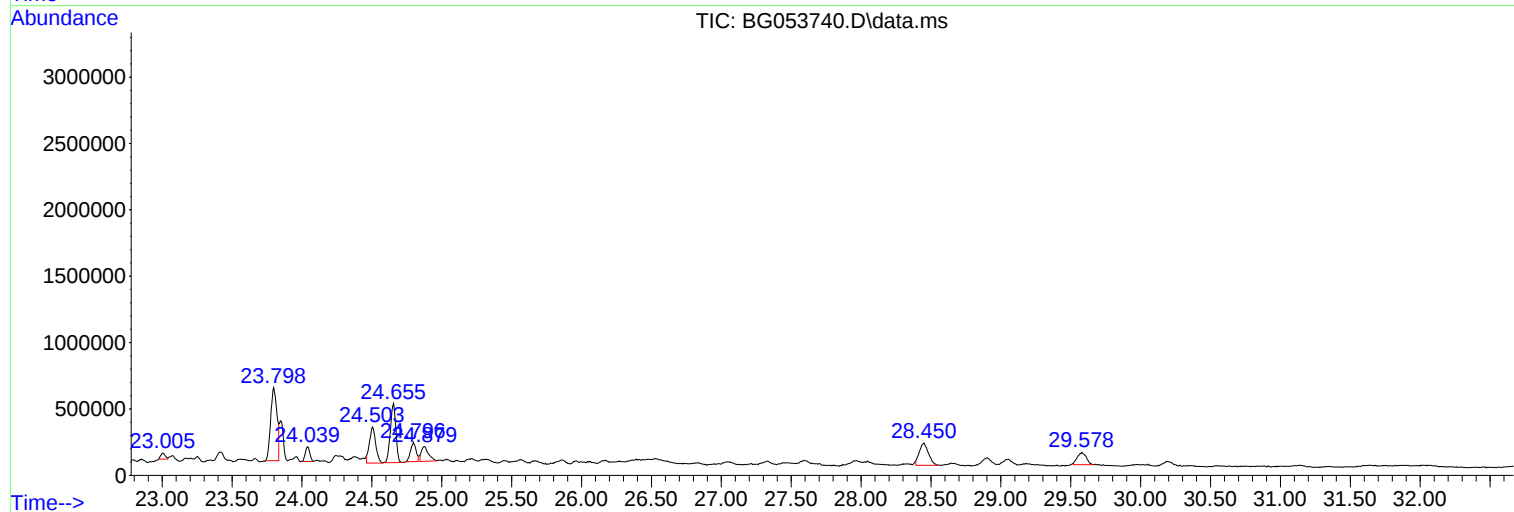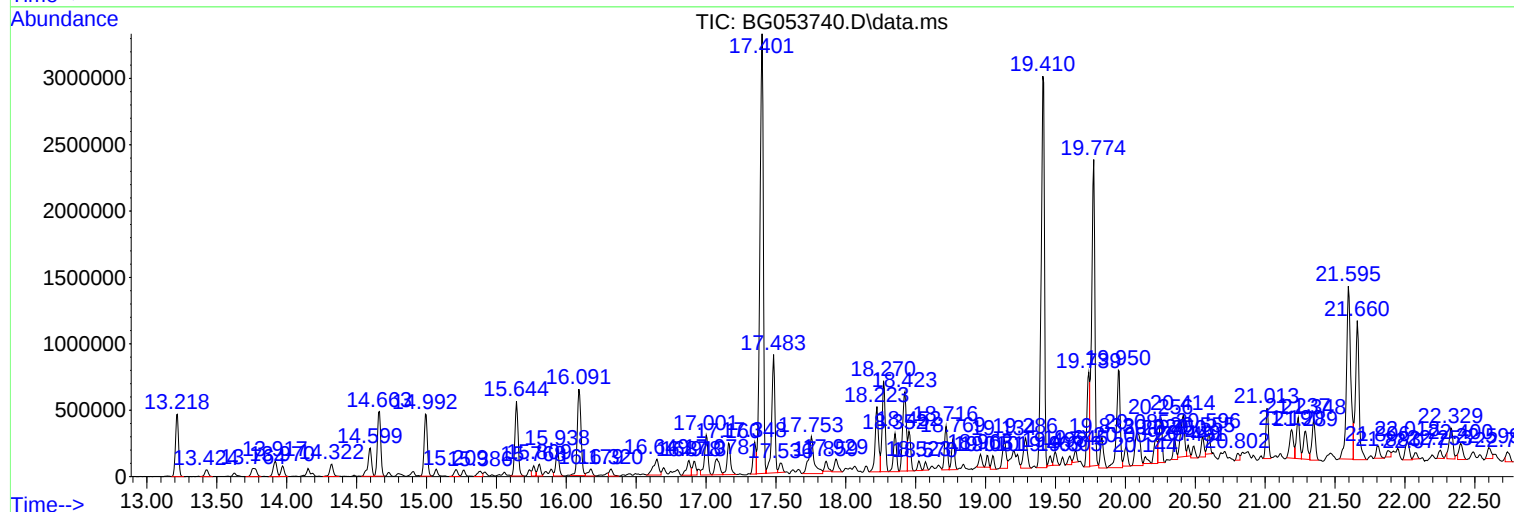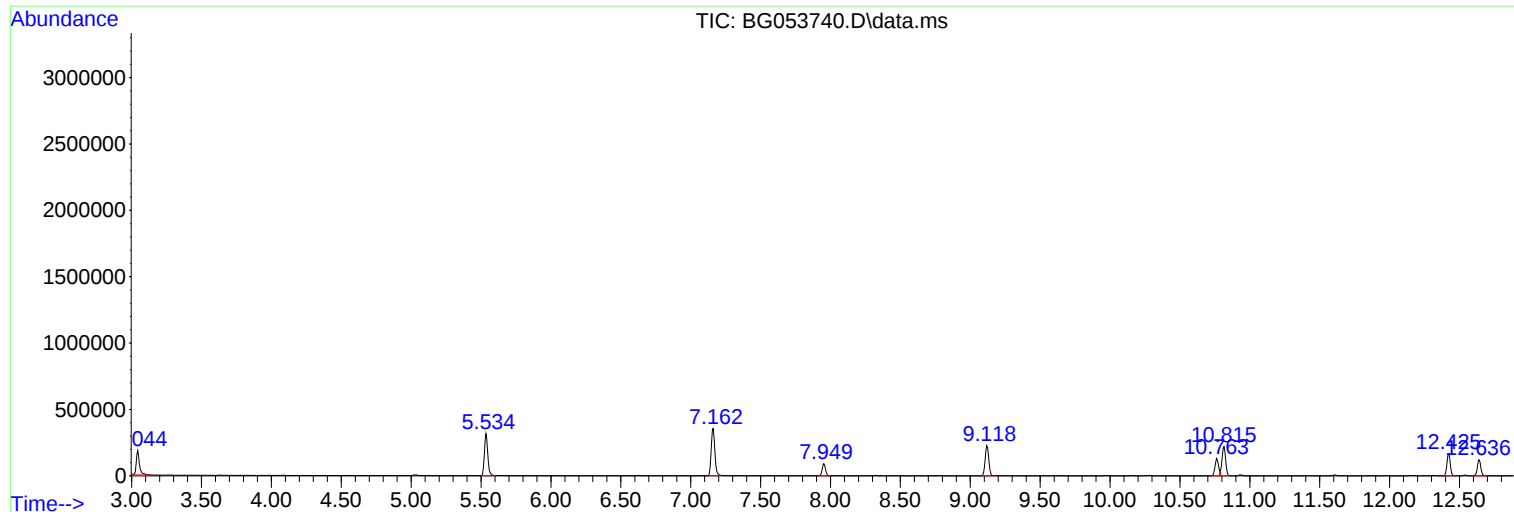

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053740.D
Acq On : 27 May 2022 19:32
Operator : CG/JU
Sample : N3072-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PSC-124035

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053740.D
Acq On : 27 May 2022 19:32
Operator : CG/JU
Sample : N3072-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PSC-124035

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------