

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053741.D
 Acq On : 27 May 2022 20:13
 Operator : CG/JU
 Sample : N3000-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-01-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.042	4	9	26	rVB	219994	347961	17.87%	1.528%
2	5.533	426	433	448	rBV	373748	628646	32.29%	2.761%
3	7.160	703	710	725	rBV	422910	737994	37.91%	3.241%
4	7.953	839	845	854	rVB	94300	156992	8.06%	0.689%
5	9.122	1036	1044	1053	rBV	261182	472853	24.29%	2.077%
6	10.761	1317	1323	1330	rBV	134644	234348	12.04%	1.029%
7	13.216	1734	1741	1750	rBV	655090	983501	50.52%	4.319%
8	14.597	1967	1976	1982	rBV	223151	350361	18.00%	1.539%
9	14.661	1982	1987	1993	rVB	36349	55648	2.86%	0.244%
10	14.990	2037	2043	2050	rBV	17347	29564	1.52%	0.130%
11	15.642	2147	2154	2161	rBV3	31800	53696	2.76%	0.236%
12	15.936	2199	2204	2211	rVB2	20067	35058	1.80%	0.154%
13	16.089	2224	2230	2240	rBV	554033	873236	44.86%	3.835%
14	16.653	2314	2326	2330	rBV6	18807	49353	2.54%	0.217%
15	16.876	2355	2364	2367	rBV3	23792	47423	2.44%	0.208%
16	16.917	2367	2371	2374	rVB2	15493	20251	1.04%	0.089%
17	16.999	2380	2385	2390	rVB3	27118	43053	2.21%	0.189%
18	17.076	2390	2398	2408	rVV6	21700	53973	2.77%	0.237%
19	17.164	2408	2413	2423	rVB	29432	51851	2.66%	0.228%
20	17.346	2438	2444	2447	rBV	256323	418219	21.48%	1.837%
21	17.387	2447	2451	2458	rVV	643177	918532	47.18%	4.034%
22	17.475	2461	2466	2471	rVB	138590	208843	10.73%	0.917%
23	17.528	2471	2475	2481	rBV4	12775	27650	1.42%	0.121%
24	17.751	2504	2513	2521	rBV4	26253	75641	3.89%	0.332%
25	17.857	2527	2531	2535	rVB	26453	34502	1.77%	0.152%
26	17.922	2538	2542	2551	rVB5	18668	39192	2.01%	0.172%
27	18.221	2586	2593	2597	rBV	113832	228092	11.72%	1.002%
28	18.268	2597	2601	2607	rVB	159387	250071	12.85%	1.098%
29	18.351	2609	2615	2620	rVV	58340	93246	4.79%	0.410%
30	18.415	2620	2626	2630	rVV2	156821	308762	15.86%	1.356%
31	18.450	2630	2632	2640	rVB	83799	108606	5.58%	0.477%
32	18.521	2640	2644	2649	rBV6	19813	31779	1.63%	0.140%
33	18.615	2655	2660	2664	rBV7	12305	20224	1.04%	0.089%
34	18.715	2672	2677	2681	rBV	89411	133081	6.84%	0.584%
35	18.762	2681	2685	2691	rVB	65508	97067	4.99%	0.426%
36	18.961	2710	2719	2723	rBV	42589	89057	4.57%	0.391%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053741.D
 Acq On : 27 May 2022 20:13
 Operator : CG/JU
 Sample : N3000-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-01-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.014	2724	2728	2731	rVV	31786	49265	2.53%	0.216%
38	19.050	2731	2734	2738	rVB2	26093	33201	1.71%	0.146%
39	19.132	2743	2748	2752	rBV	75200	139511	7.17%	0.613%
40	19.279	2768	2773	2781	rVB2	72857	131541	6.76%	0.578%
41	19.402	2787	2794	2800	rBV	1372420	1946725	100.00%	8.549%
42	19.461	2800	2804	2806	rVV	19895	23512	1.21%	0.103%
43	19.502	2806	2811	2816	rVV4	38802	78049	4.01%	0.343%
44	19.596	2823	2827	2830	rBV3	17060	25102	1.29%	0.110%
45	19.643	2831	2835	2839	rVV	42700	55507	2.85%	0.244%
46	19.731	2845	2850	2851	rBV	238483	303311	15.58%	1.332%
47	19.766	2851	2856	2863	rVV	1230745	1801455	92.54%	7.912%
48	19.831	2863	2867	2874	rVB3	69437	119449	6.14%	0.525%
49	19.954	2881	2888	2893	rBV	963744	1274171	65.45%	5.596%
50	20.001	2893	2896	2901	rVB2	57033	86603	4.45%	0.380%
51	20.095	2904	2912	2916	rBV3	87143	220386	11.32%	0.968%
52	20.219	2928	2933	2934	rBV3	66100	99892	5.13%	0.439%
53	20.254	2935	2939	2943	rVB	144696	220203	11.31%	0.967%
54	20.348	2952	2955	2959	rBV	76109	107925	5.54%	0.474%
55	20.412	2959	2966	2970	rVV2	107618	198385	10.19%	0.871%
56	20.548	2985	2989	2993	rBV	77645	118912	6.11%	0.522%
57	20.595	2994	2997	3001	rVB2	77561	94005	4.83%	0.413%
58	21.012	3064	3068	3074	rVB	116428	165905	8.52%	0.729%
59	21.188	3093	3098	3102	rBV2	86500	164963	8.47%	0.724%
60	21.235	3102	3106	3110	rVV2	126400	215292	11.06%	0.946%
61	21.282	3110	3114	3119	rVV2	105055	186845	9.60%	0.821%
62	21.341	3120	3124	3130	rVB	110044	182146	9.36%	0.800%
63	21.593	3157	3167	3173	rBV2	652448	1556067	79.93%	6.834%
64	21.652	3173	3177	3190	rVB	509450	913625	46.93%	4.012%
65	21.805	3198	3203	3210	rBV2	89002	166460	8.55%	0.731%
66	22.328	3288	3292	3297	rVB	86181	144090	7.40%	0.633%
67	23.790	3532	3541	3547	rBV	345758	1078811	55.42%	4.738%
68	24.037	3579	3583	3591	rVB	70871	149531	7.68%	0.657%
69	24.501	3655	3662	3676	rVB	210094	643450	33.05%	2.826%
70	24.648	3678	3687	3698	rVB	313190	860458	44.20%	3.779%
71	24.795	3705	3712	3719	rBV2	127533	340597	17.50%	1.496%
72	28.437	4323	4332	4347	rVB3	124824	566386	29.09%	2.487%


Sum of corrected areas: 22770062

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053741.D
Acq On : 27 May 2022 20:13
Operator : CG/JU
Sample : N3000-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-01-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

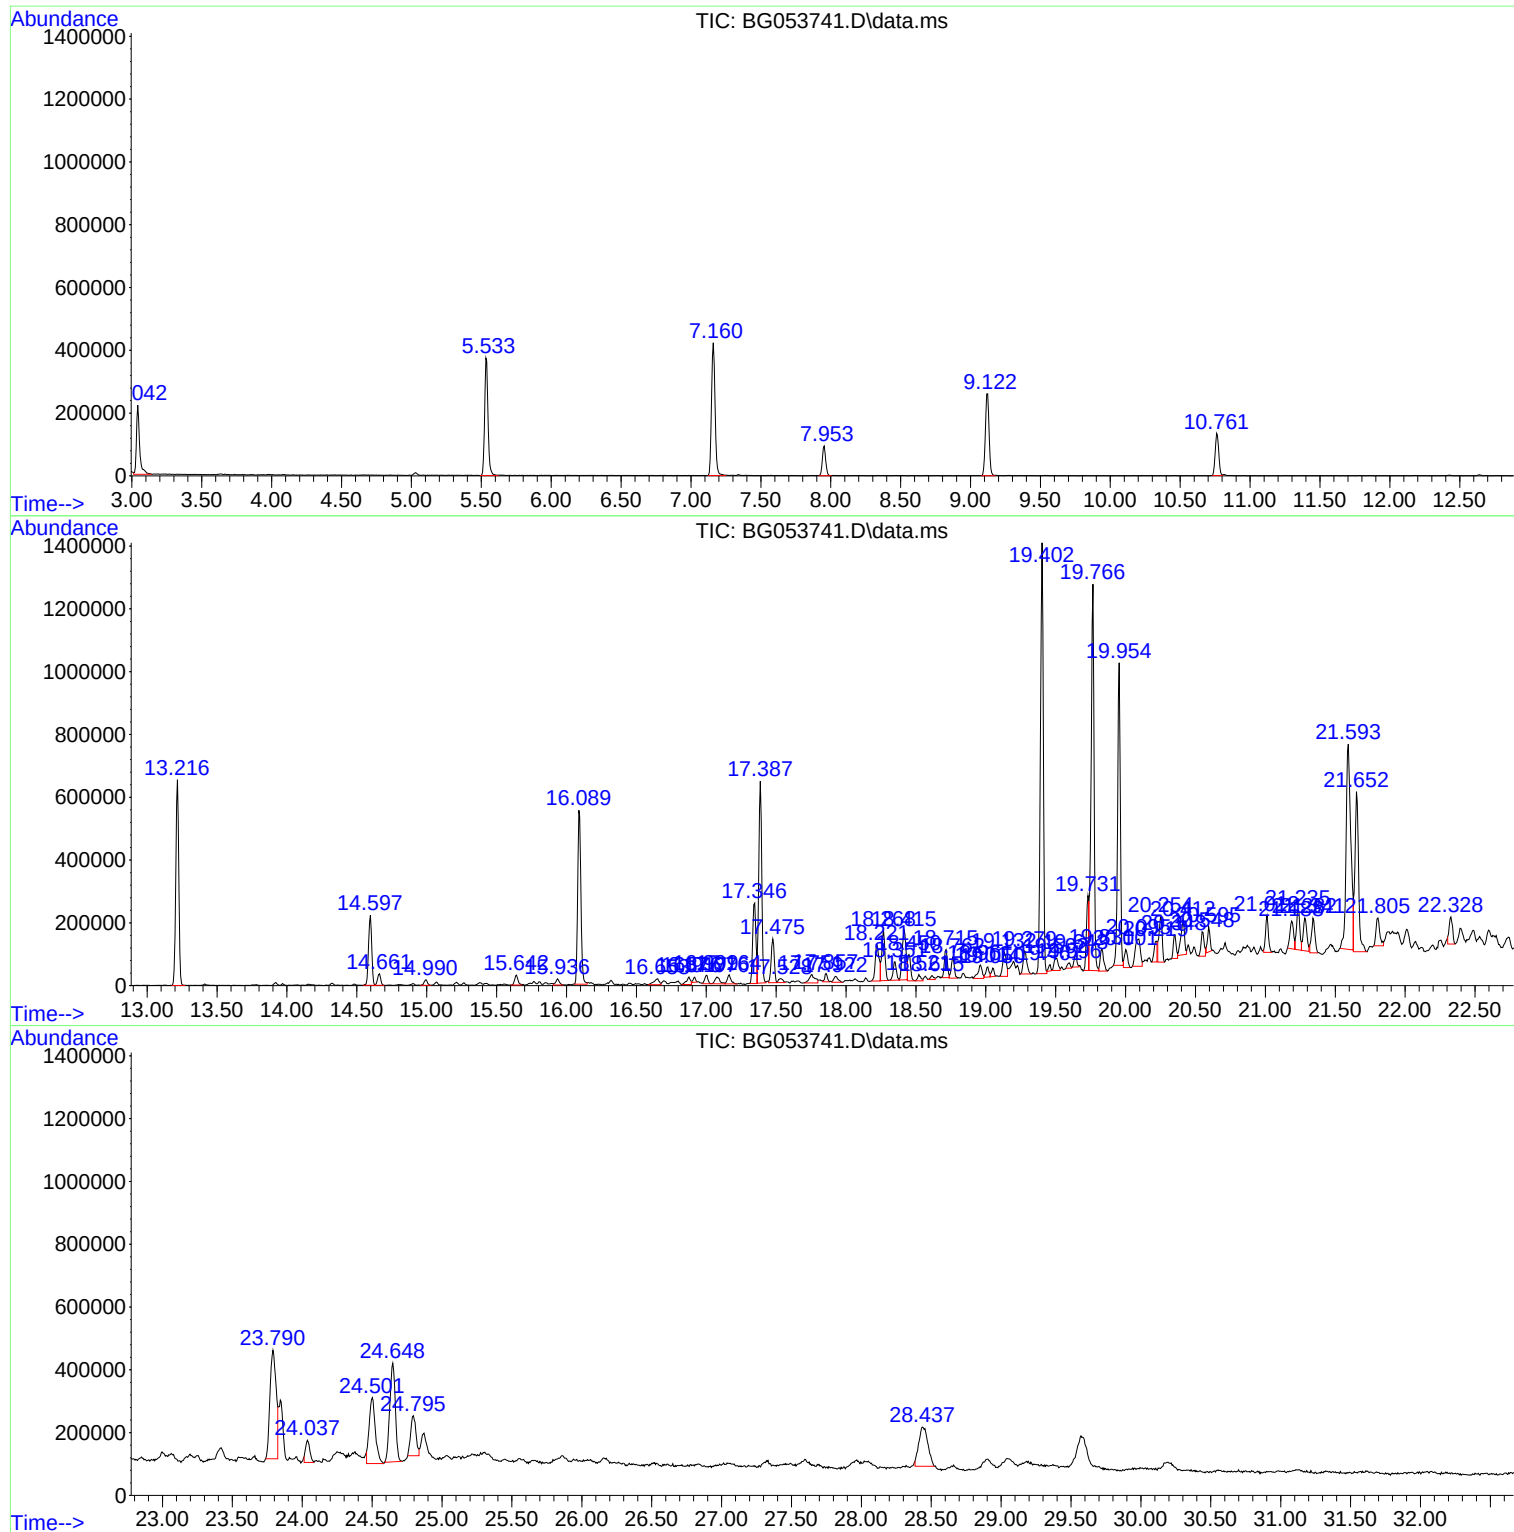

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053741.D
Acq On : 27 May 2022 20:13
Operator : CG/JU
Sample : N3000-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-01-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053741.D
Acq On : 27 May 2022 20:13
Operator : CG/JU
Sample : N3000-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-01-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------