

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053743.D
 Acq On : 27 May 2022 21:33
 Operator : CG/JU
 Sample : N3070-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 IG1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053743.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.041	4	9	23	rVB	200474	324467	23.55%	2.478%
2	5.032	343	348	352	rBV3	9438	15821	1.15%	0.121%
3	5.537	427	434	446	rBV	394298	666468	48.37%	5.091%
4	7.159	703	710	723	rBV	455431	796418	57.81%	6.083%
5	7.952	838	845	852	rBV	106844	174389	12.66%	1.332%
6	9.121	1036	1044	1053	rBV	292497	514769	37.36%	3.932%
7	10.765	1314	1324	1330	rBV	141726	254009	18.44%	1.940%
8	13.215	1734	1741	1754	rBV	747948	1138129	82.61%	8.693%
9	14.325	1925	1930	1935	rBV2	10151	17193	1.25%	0.131%
10	14.596	1965	1976	1982	rBV	231851	361891	26.27%	2.764%
11	14.660	1982	1987	1992	rVB	14431	22977	1.67%	0.176%
12	14.995	2039	2044	2049	rVB3	9303	15853	1.15%	0.121%
13	15.641	2149	2154	2165	rVB2	19956	37198	2.70%	0.284%
14	16.094	2225	2231	2239	rBV	578737	894030	64.89%	6.829%
15	16.323	2267	2270	2275	rVB5	12508	17924	1.30%	0.137%
16	16.699	2329	2334	2339	rVB4	9244	14726	1.07%	0.112%
17	16.875	2356	2364	2368	rBV8	7172	14960	1.09%	0.114%
18	16.939	2368	2375	2380	rVV3	17766	33133	2.40%	0.253%
19	17.086	2395	2400	2403	rVB6	10055	14460	1.05%	0.110%
20	17.163	2405	2413	2421	rVB	18992	38731	2.81%	0.296%
21	17.257	2424	2429	2433	rBV4	15557	25933	1.88%	0.198%
22	17.345	2437	2444	2447	rBV	264867	407210	29.56%	3.110%
23	17.386	2447	2451	2461	rVV	225790	337031	24.46%	2.574%
24	17.474	2461	2466	2471	rVB	34749	54458	3.95%	0.416%
25	17.539	2471	2477	2482	rBV6	12738	24824	1.80%	0.190%
26	17.715	2501	2507	2510	rBV3	11938	23081	1.68%	0.176%
27	17.756	2510	2514	2521	rVB2	16135	29150	2.12%	0.223%
28	17.926	2536	2543	2551	rVB2	23862	47767	3.47%	0.365%
29	18.073	2564	2568	2572	rVB3	12743	22217	1.61%	0.170%
30	18.132	2572	2578	2584	rBV9	10355	26855	1.95%	0.205%
31	18.238	2587	2596	2599	rVV4	99448	221353	16.07%	1.691%
32	18.267	2599	2601	2607	rVV	83635	108850	7.90%	0.831%
33	18.349	2610	2615	2620	rBV	16977	28069	2.04%	0.214%
34	18.414	2620	2626	2630	rBV2	83795	158148	11.48%	1.208%
35	18.449	2630	2632	2638	rVB2	42590	58128	4.22%	0.444%
36	18.614	2656	2660	2666	rBV5	14813	26701	1.94%	0.204%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053743.D
 Acq On : 27 May 2022 21:33
 Operator : CG/JU
 Sample : N3070-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 IG1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.714	2673	2677	2681	rBV2	39335	55734	4.05%	0.426%
38	18.766	2681	2686	2695	rVB2	37666	70732	5.13%	0.540%
39	18.943	2712	2716	2717	rBV4	12151	17605	1.28%	0.134%
40	19.013	2725	2728	2731	rBV	22515	27253	1.98%	0.208%
41	19.048	2732	2734	2738	rVB3	14483	17063	1.24%	0.130%
42	19.137	2744	2749	2753	rBV	53926	88990	6.46%	0.680%
43	19.189	2753	2758	2762	rVV5	18838	40002	2.90%	0.306%
44	19.277	2768	2773	2779	rBV3	27141	66580	4.83%	0.509%
45	19.401	2788	2794	2799	rBV	437946	632898	45.94%	4.834%
46	19.512	2807	2813	2817	rBV7	27065	63623	4.62%	0.486%
47	19.636	2832	2834	2838	rVB2	22279	25324	1.84%	0.193%
48	19.730	2845	2850	2851	rBV	71007	91295	6.63%	0.697%
49	19.759	2851	2855	2863	rVV	394411	596577	43.30%	4.557%
50	19.836	2864	2868	2874	rVB2	32903	46940	3.41%	0.359%
51	19.953	2882	2888	2894	rBV	1073118	1377752	100.00%	10.524%
52	20.253	2936	2939	2944	rVB	93301	123779	8.98%	0.945%
53	20.353	2952	2956	2960	rBV	54820	74598	5.41%	0.570%
54	20.411	2963	2966	2970	rVB	43222	58307	4.23%	0.445%
55	20.552	2986	2990	2994	rBV	45112	63947	4.64%	0.488%
56	20.593	2994	2997	3002	rVV	44479	63405	4.60%	0.484%
57	21.193	3096	3099	3102	rBV	33977	42067	3.05%	0.321%
58	21.240	3102	3107	3111	rBV2	157400	222404	16.14%	1.699%
59	21.604	3162	3169	3174	rBV2	294379	691351	50.18%	5.281%
60	21.651	3174	3177	3183	rVB	155835	230880	16.76%	1.764%
61	21.809	3200	3204	3210	rVB3	75275	115201	8.36%	0.880%
62	21.874	3212	3215	3220	rVB2	91025	130646	9.48%	0.998%
63	23.789	3534	3541	3546	rBV2	98875	278829	20.24%	2.130%
64	24.500	3658	3662	3676	rVB	79914	201360	14.62%	1.538%
65	24.641	3681	3686	3696	rVB2	105541	279363	20.28%	2.134%
66	24.794	3705	3712	3720	rVB	129898	329972	23.95%	2.520%


Sum of corrected areas: 13091798

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053743.D
Acq On : 27 May 2022 21:33
Operator : CG/JU
Sample : N3070-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
IG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

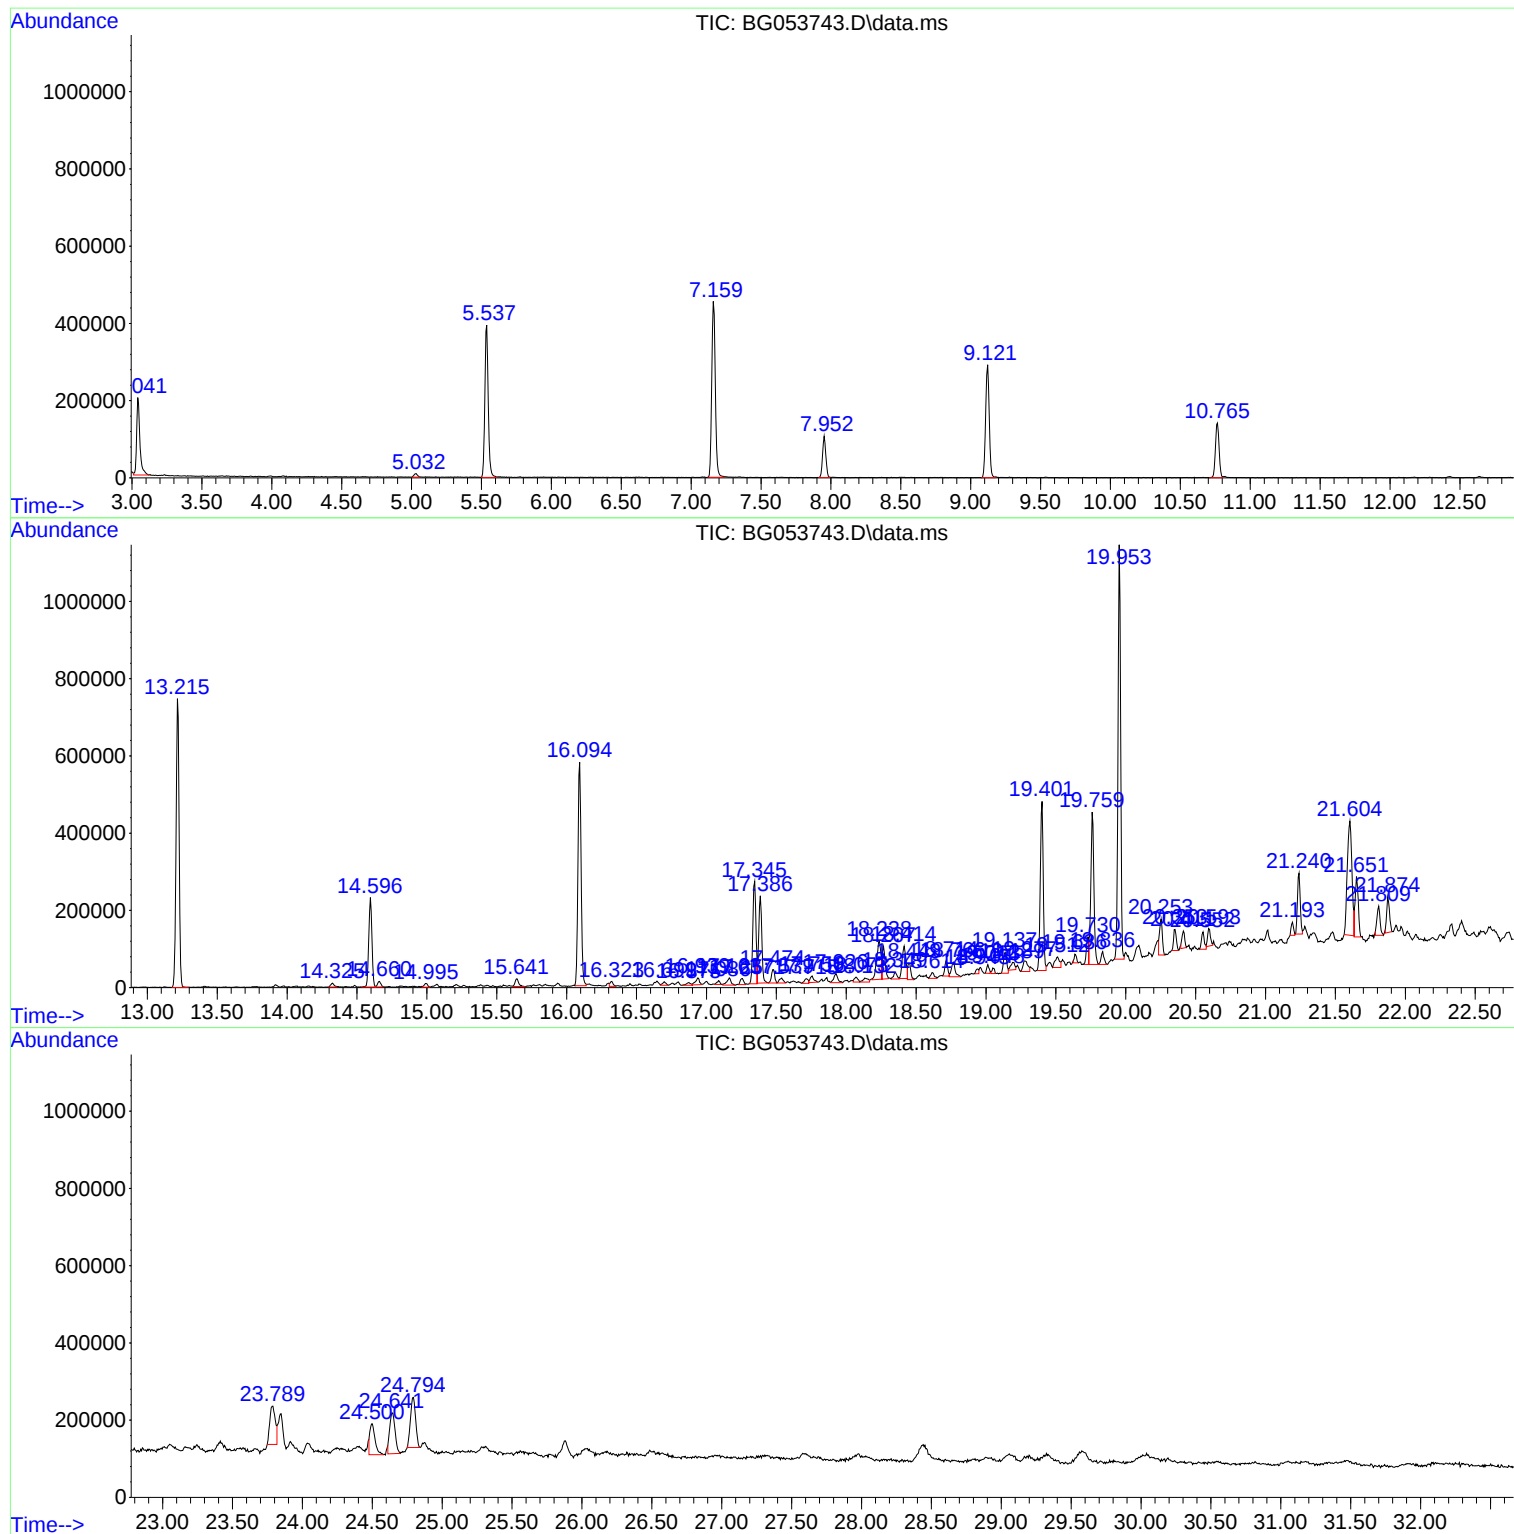

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053743.D
Acq On : 27 May 2022 21:33
Operator : CG/JU
Sample : N3070-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
IG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053743.D
Acq On : 27 May 2022 21:33
Operator : CG/JU
Sample : N3070-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
IG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc