
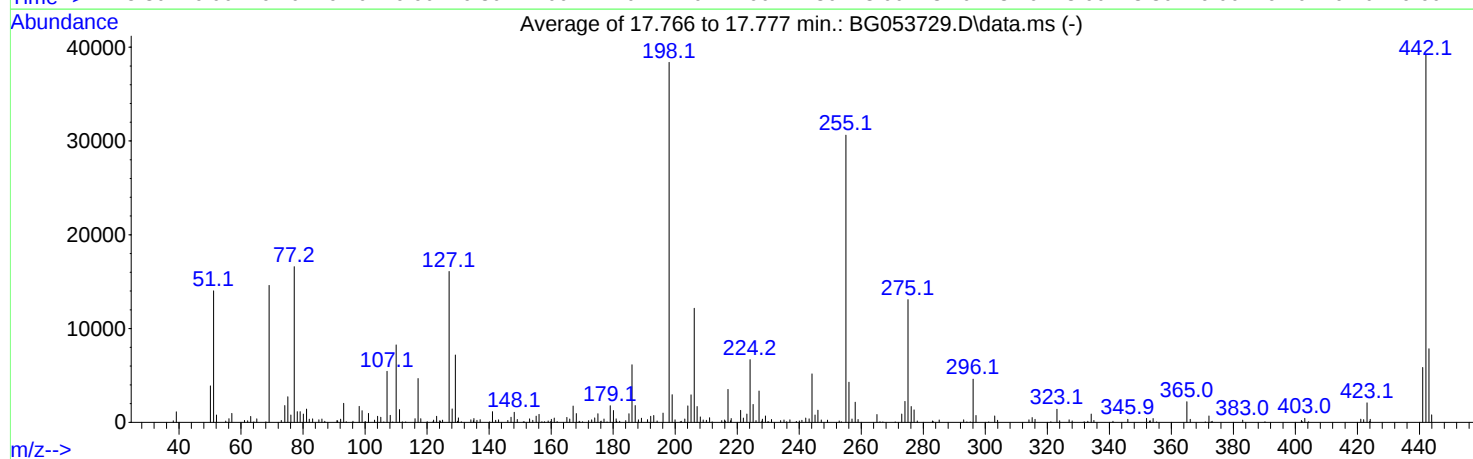


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
 Data File : BG053729.D
 Acq On : 27 May 2022 11:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun May 29 02:17:06 2022

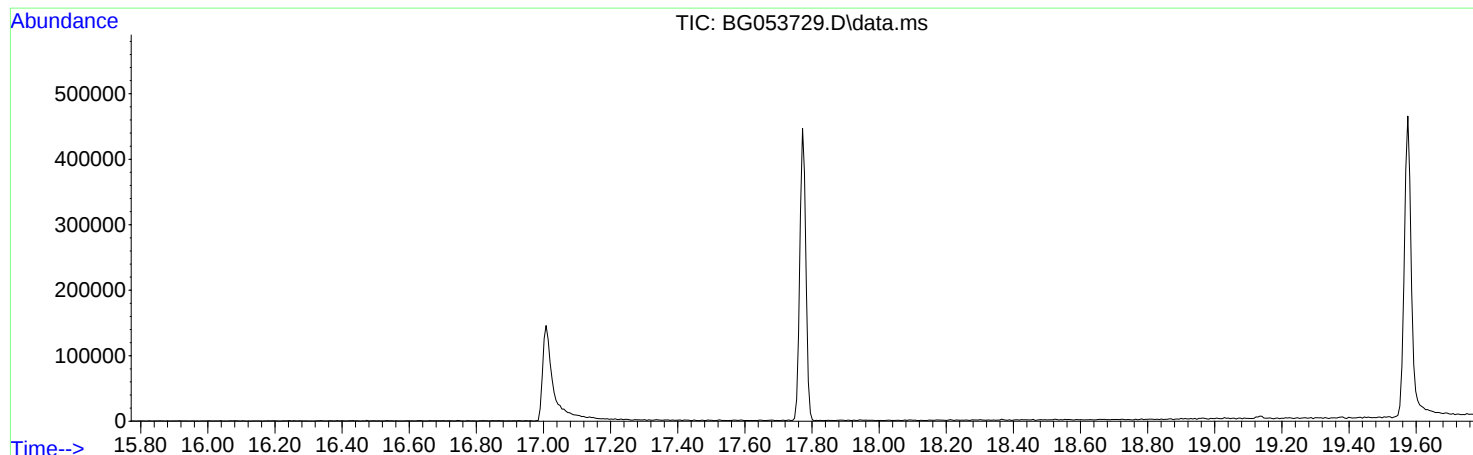

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	14026	PASS
68	69	0.00	2	0.4	59	PASS
69	198	0.00	100	38.1	14605	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.9	16093	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38381	PASS
199	198	5	9	7.7	2952	PASS
275	198	10	60	34.1	13086	PASS
365	198	1	100	5.8	2207	PASS
441	198	0.01	100	15.2	5852	PASS
442	442	50	100	100.0	39221	PASS
443	442	15	24	20.0	7854	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/27/2022	BNA_G	<u>BG053729.D</u>
Compound Name	Response	Retention Time
DDT	146886	20.803
DDD	1859	20.421
DDE	275	19.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2134	149020	1.43

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053729.D
Acq On : 27 May 2022 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 28 06:39:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

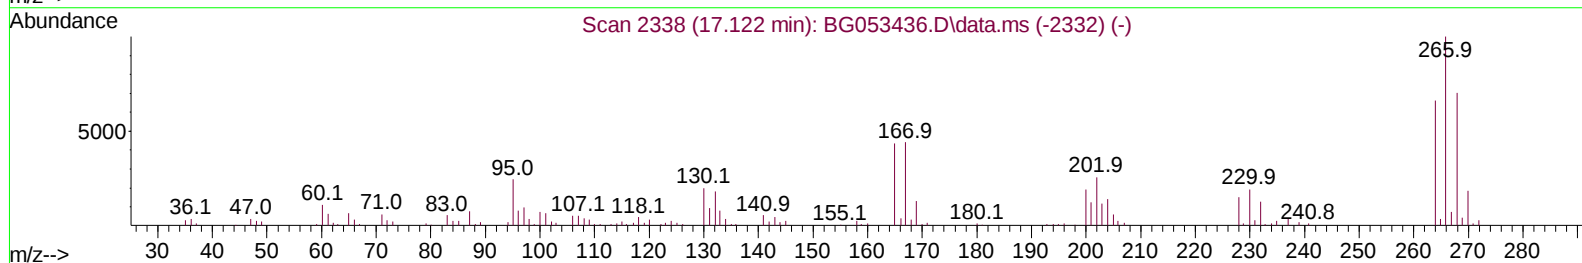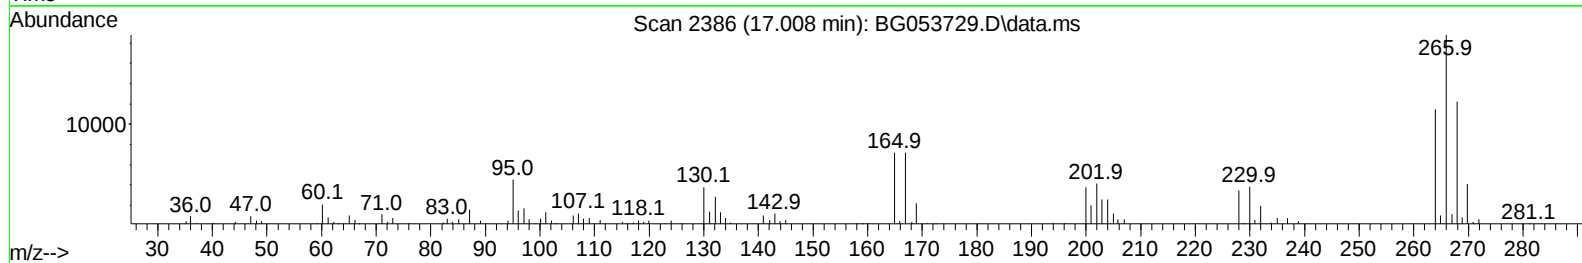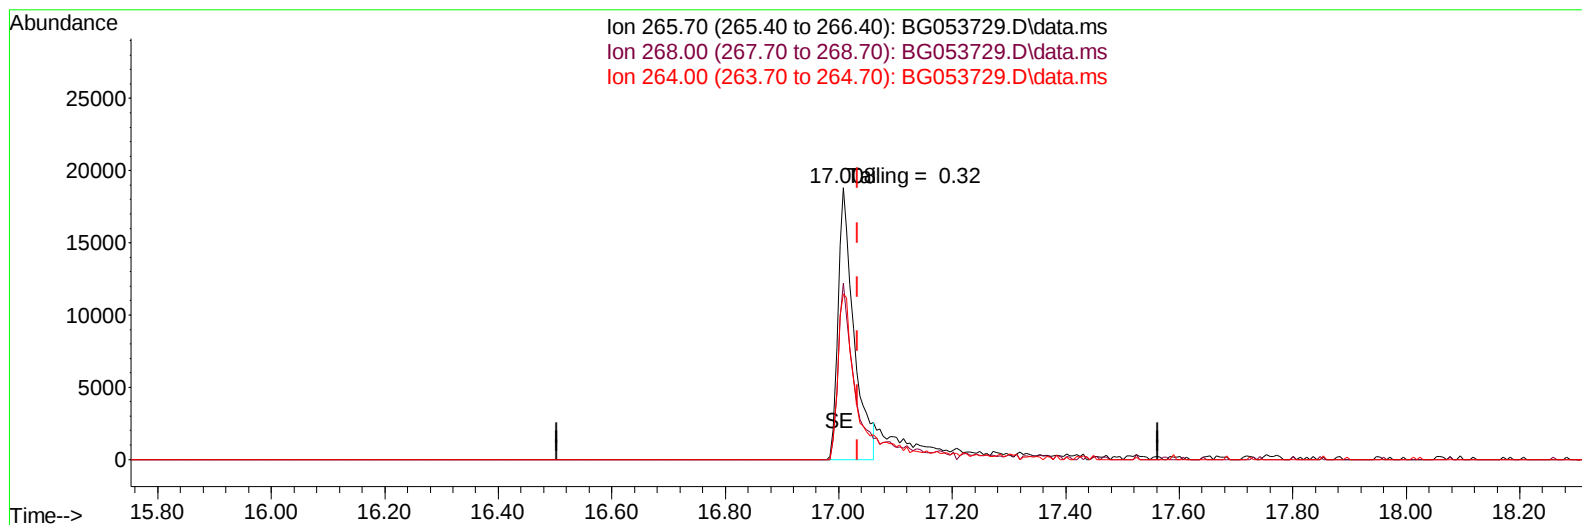

TIC: BG053729.D\data.ms

(70) Pentachlorophenol (C)

17.008min (-0.025) 18456.81 ng




response 38864

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.07
264.00	66.20	61.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052722\
Data File : BG053729.D
Acq On : 27 May 2022 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 27 11:57:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

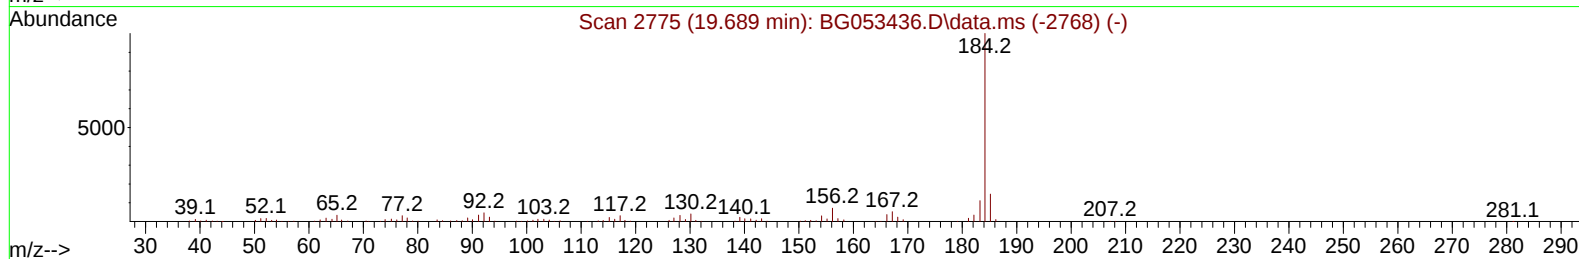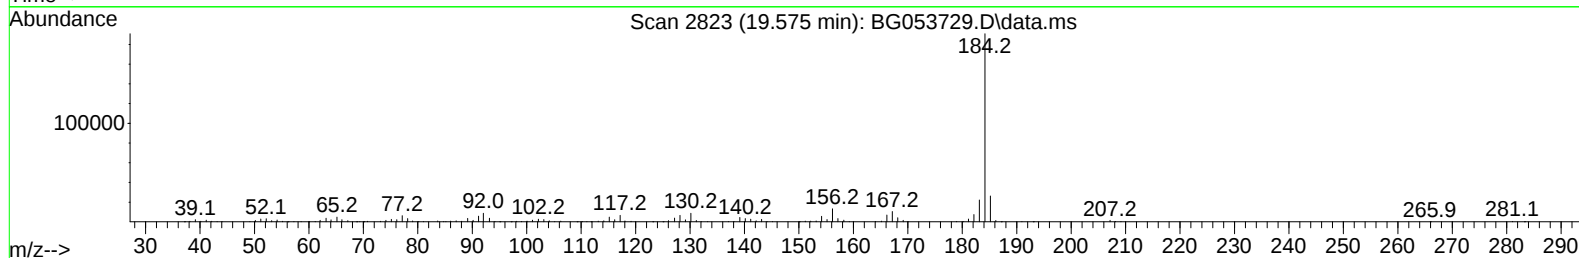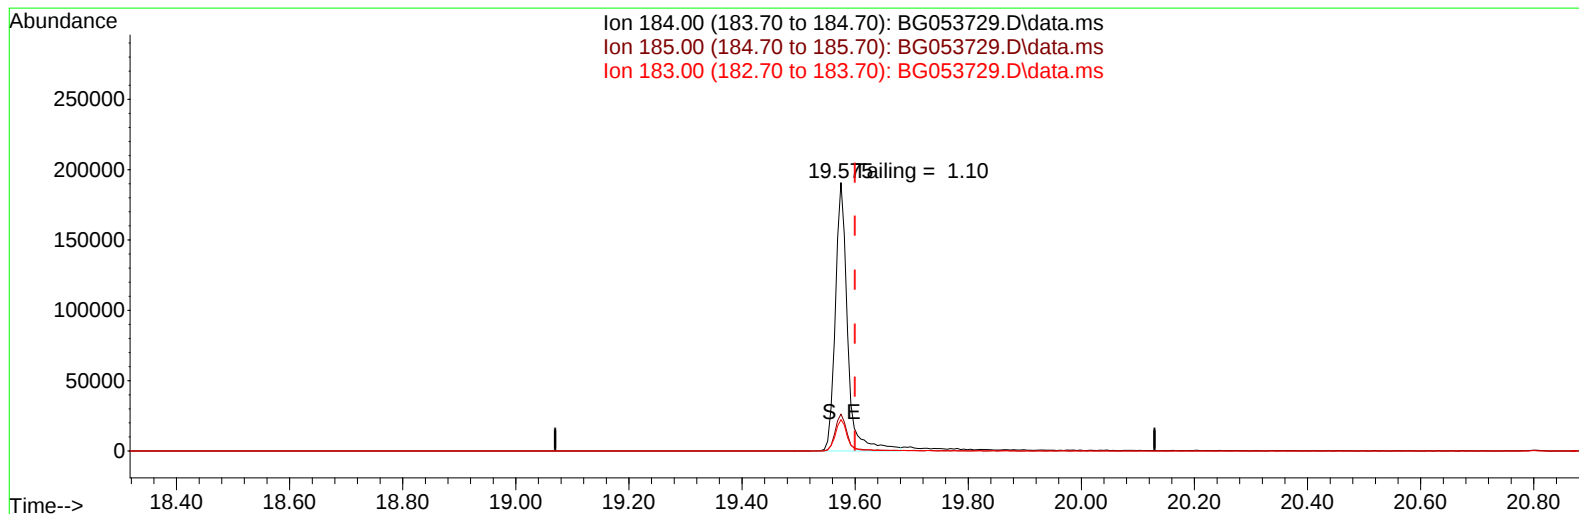

TIC: BG053729.D\data.ms

(77) Benzidine

19.575min (-0.025) 0.00 ng

response 287731

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.79
183.00	11.10	11.68
0.00	0.00	0.00