
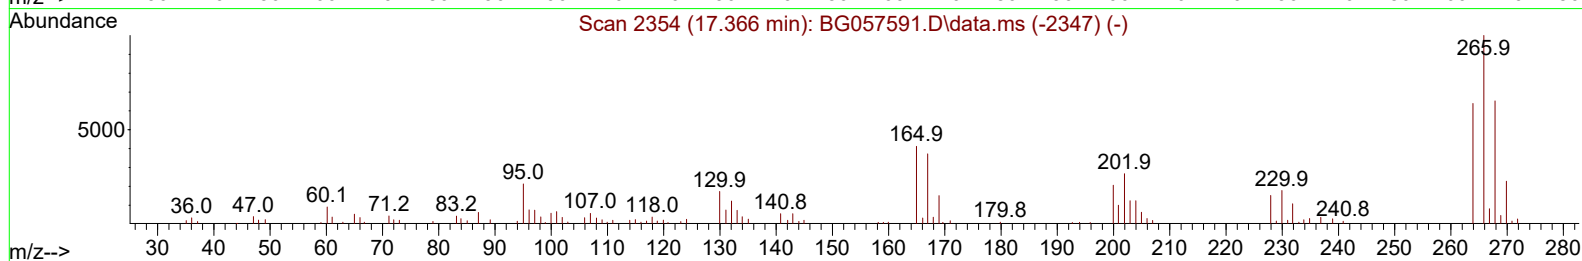
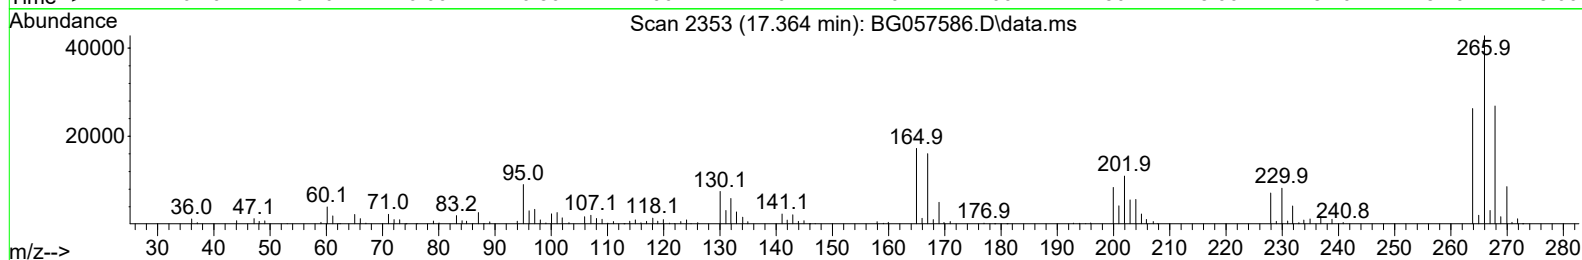


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052723\
Data File : BG057586.D
Acq On : 26 May 2023 16:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 06:37:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 23:44:40 2023
Response via : Initial Calibration

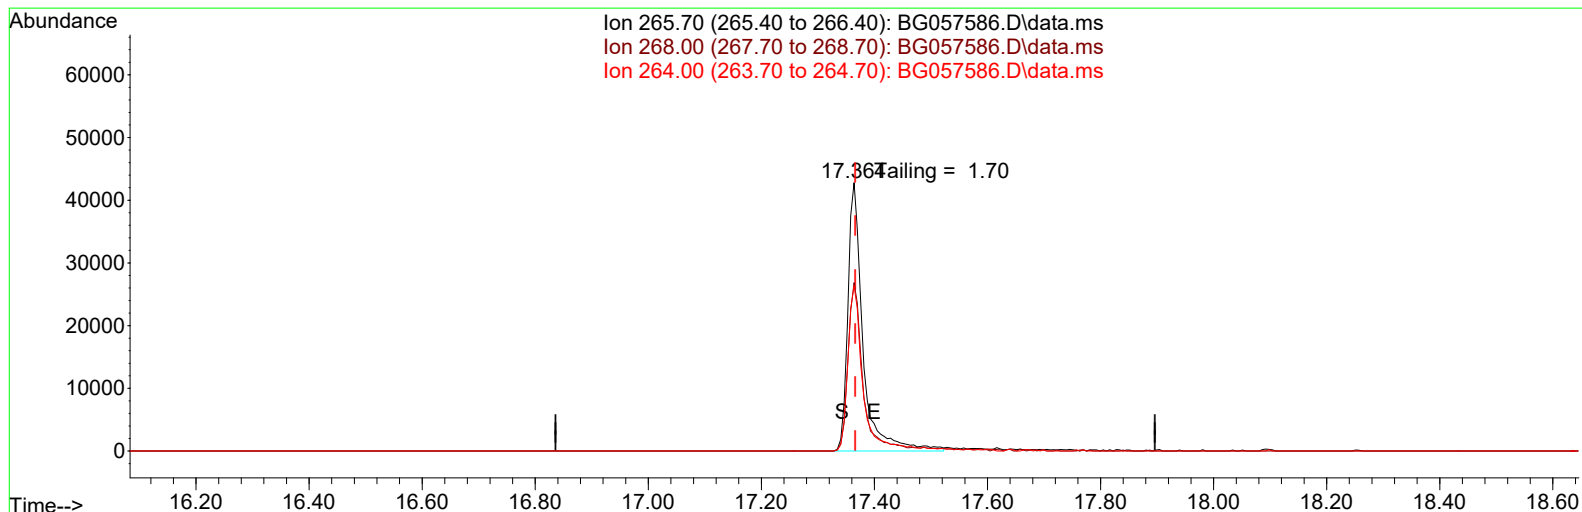

TIC: BG057586.D\data.ms

(70) Pentachlorophenol (C)




17.364min (-0.002) 38955.20 ng

response 78493

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.75
264.00	64.00	61.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052723\
Data File : BG057586.D
Acq On : 26 May 2023 16:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 06:37:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 23:44:40 2023
Response via : Initial Calibration

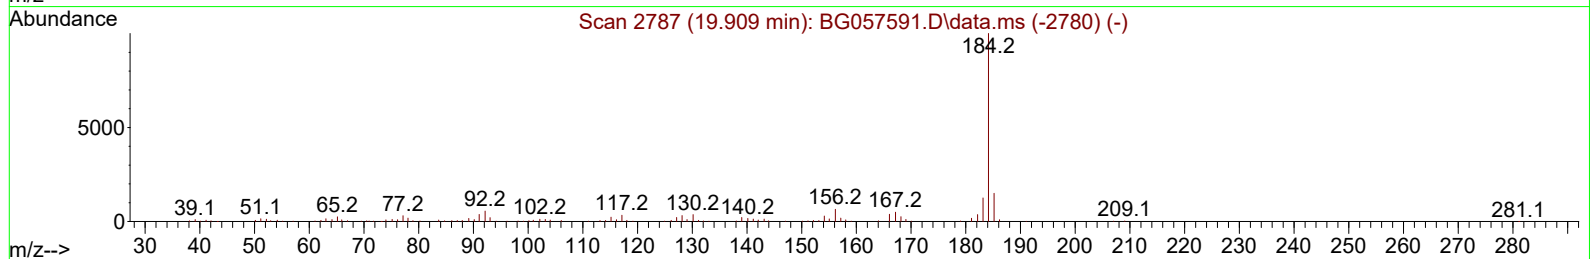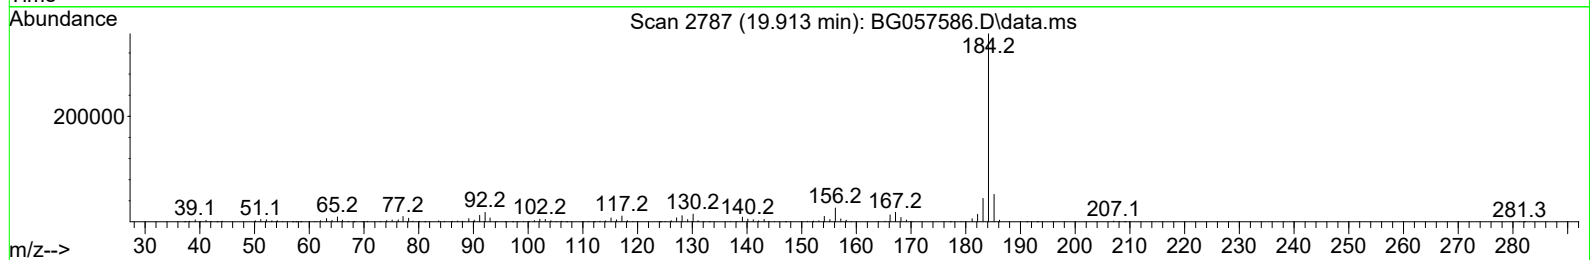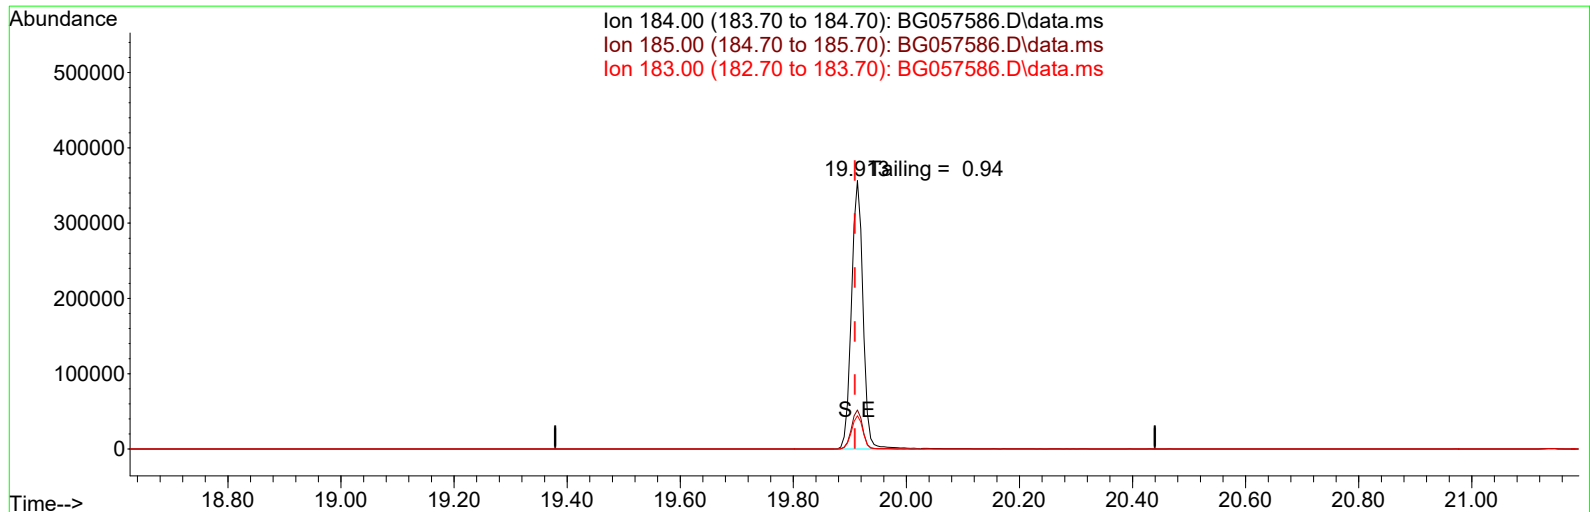

TIC: BG057586.D\data.ms

(77) Benzidine**19.913min (+ 0.004) 0.00 ng****response 505296**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.58
183.00	12.50	12.43
0.00	0.00	0.00