

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052723\
 Data File : BG057599.D
 Acq On : 27 May 2023 1:20
 Operator : CG/JU
 Sample : PB153078BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB153078BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.370	306	312	321	rBV	18155	28756	1.37%	0.438%
2	5.864	390	396	408	rBV	294266	480220	22.90%	7.316%
3	7.491	665	673	690	rBV	300223	540079	25.76%	8.228%
4	8.343	812	818	826	rVB	49425	81382	3.88%	1.240%
5	9.529	1012	1020	1028	rBV	168434	314841	15.02%	4.797%
6	11.186	1295	1302	1310	rBV	67371	120184	5.73%	1.831%
7	13.589	1704	1711	1724	rBV	561065	851768	40.62%	12.977%
8	14.963	1939	1945	1956	rBV	119774	197222	9.41%	3.005%
9	16.449	2191	2198	2217	rBV	452059	717731	34.23%	10.935%
10	17.706	2406	2412	2421	rBV	208817	312658	14.91%	4.763%
11	20.279	2843	2850	2856	rBV	1561980	2096701	100.00%	31.944%
12	22.018	3139	3146	3153	rBV2	237634	410208	19.56%	6.250%
13	25.519	3731	3742	3755	rVB	137526	411936	19.65%	6.276%




Sum of corrected areas: 6563686

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052723\
Data File : BG057599.D
Acq On : 27 May 2023 1:20
Operator : CG/JU
Sample : PB153078BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153078BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

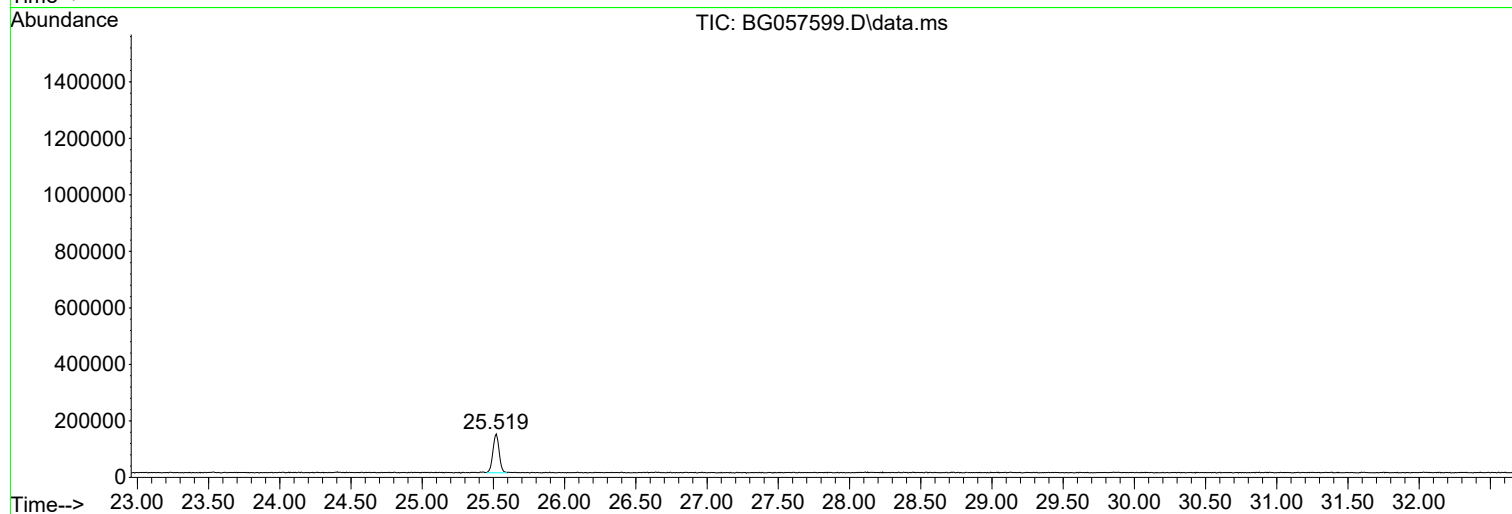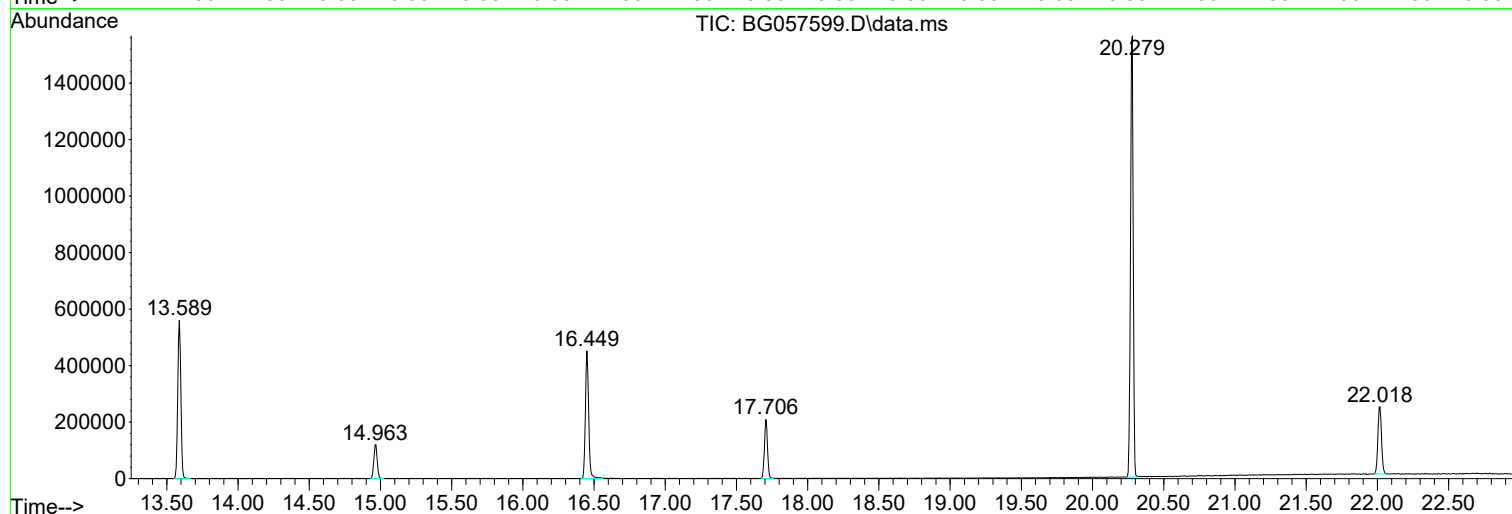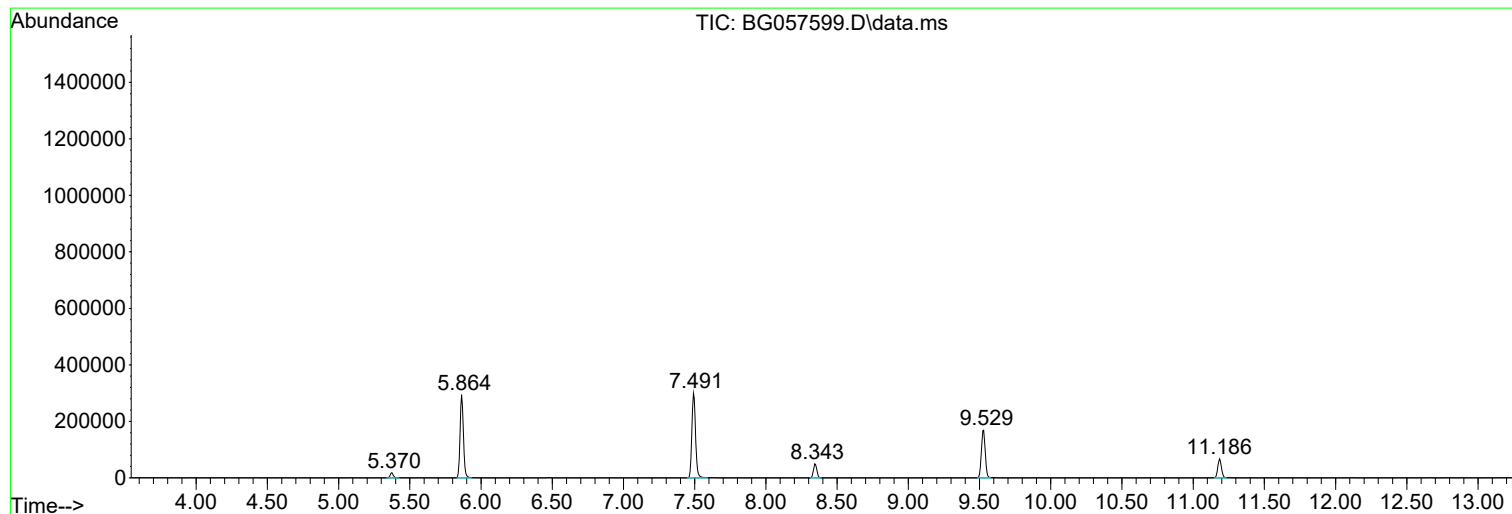

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052723\
Data File : BG057599.D
Acq On : 27 May 2023 1:20
Operator : CG/JU
Sample : PB153078BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153078BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.370	7.07 ng	28756	1,4-Dichlorobenzene-d4	8.349

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	3-Octanol	130	C8H18O	000589-98-0	36		
3	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
4	Propylamine	59	C3H9N	000107-10-8	9		
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		

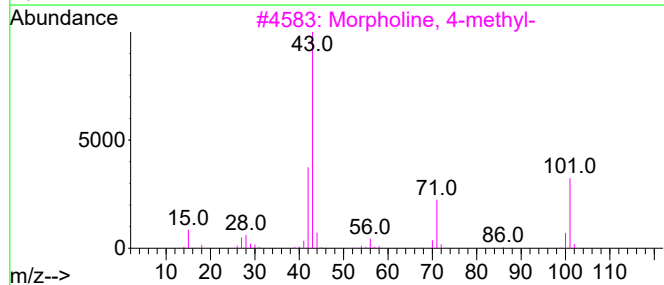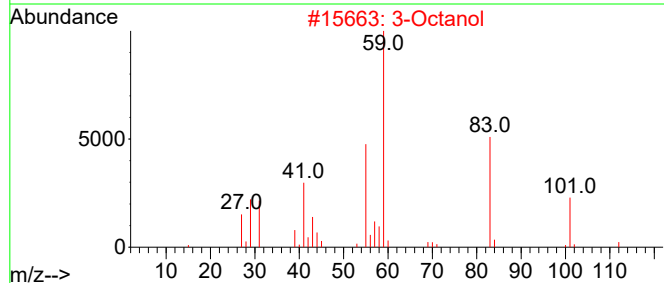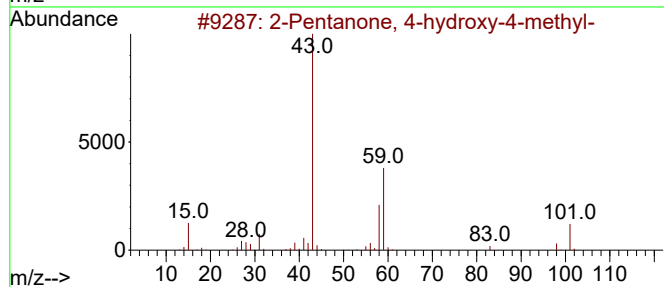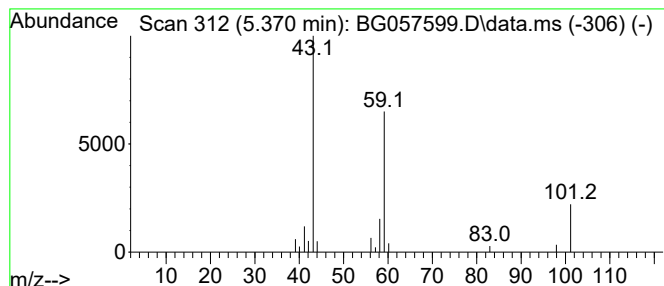

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052723\
Data File : BG057599.D
Acq On : 27 May 2023 1:20
Operator : CG/JU
Sample : PB153078BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153078BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.370	7.1	ng	28756	1	8.349	81382	20.0