


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052723\
Data File : BG057586.D
Acq On : 26 May 2023 16:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 26 23:44:40 2023

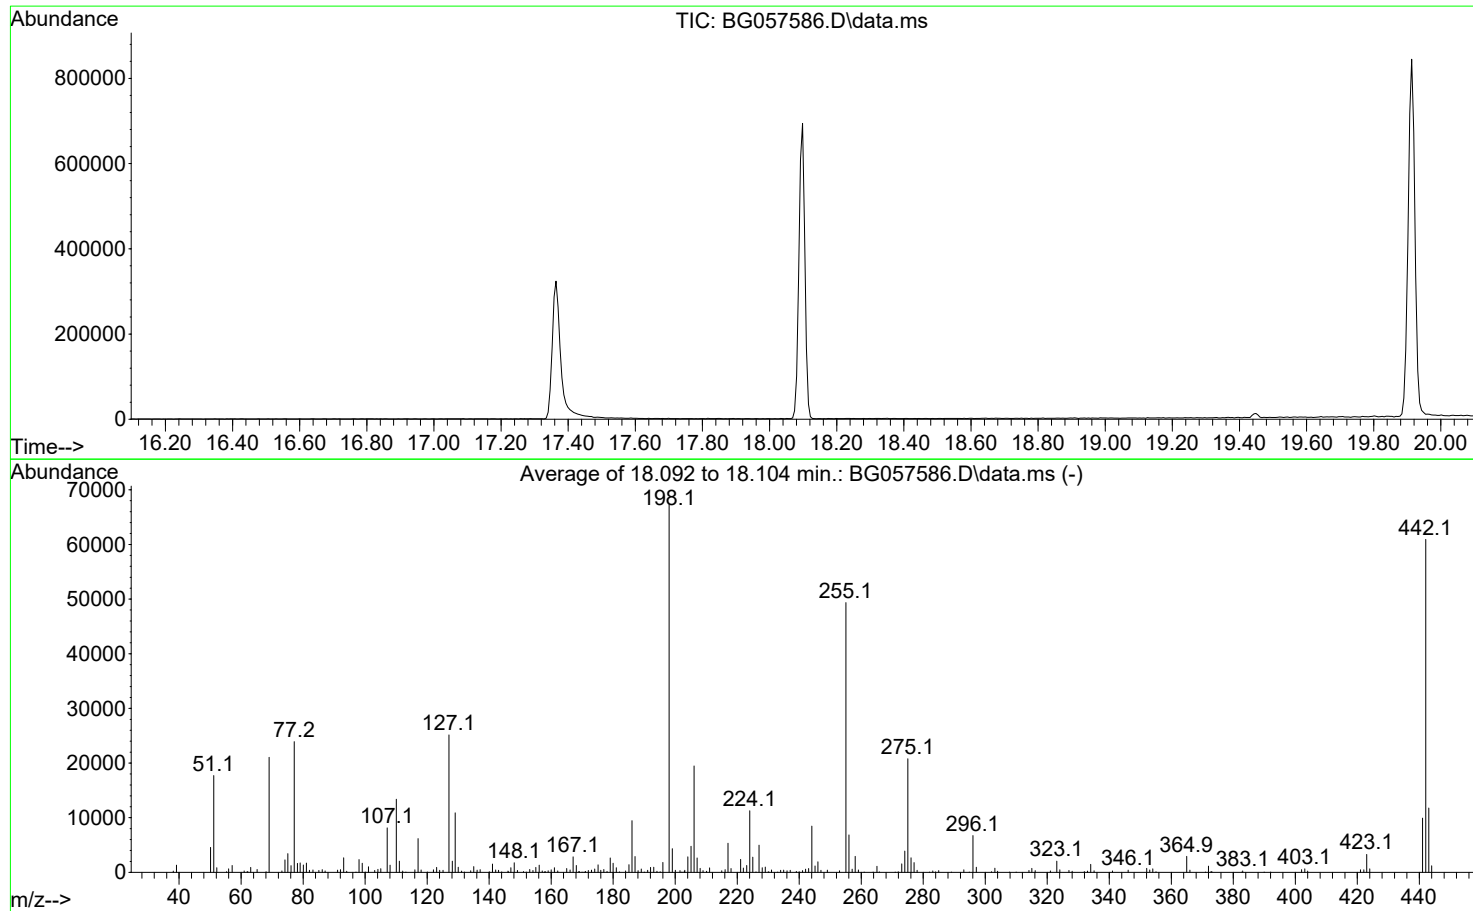

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.3	17716	PASS
68	69	0.00	2	0.5	115	PASS
69	198	0.00	100	31.3	21058	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.4	25152	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67309	PASS
199	198	5	9	6.4	4322	PASS
275	198	10	60	30.9	20792	PASS
365	198	1	100	4.3	2925	PASS
441	198	0.01	100	14.7	9925	PASS
442	442	50	100	100.0	60923	PASS
443	442	15	24	19.3	11782	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/27/2023	BNA_G	<u>BG057586.D</u>
Compound Name	Response	Retention Time
DDT	237600	21.141
DDD	4383	20.732
DDE	582	20.184
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4965	242565	2.05

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052723\
Data File : BG057586.D
Acq On : 26 May 2023 16:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 27 06:37:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 23:44:40 2023
Response via : Initial Calibration

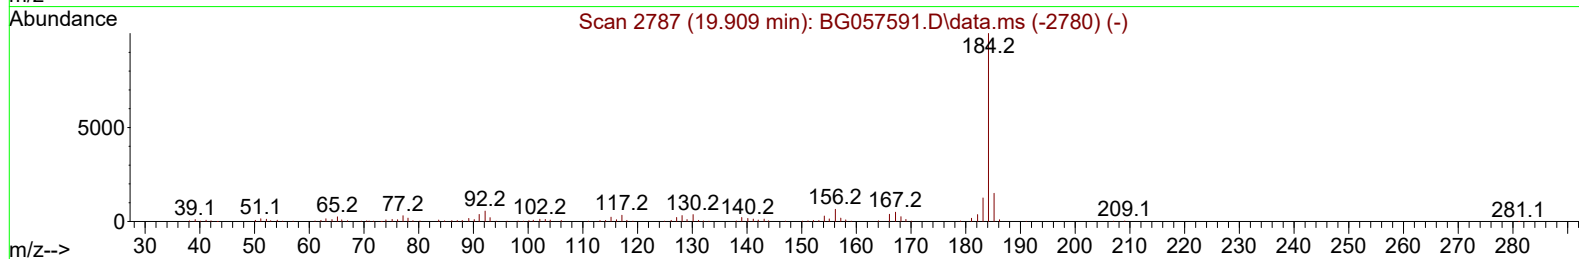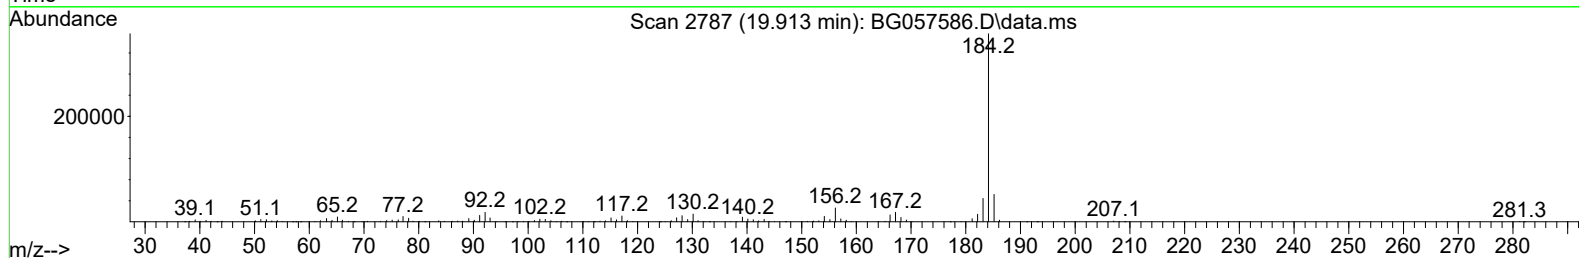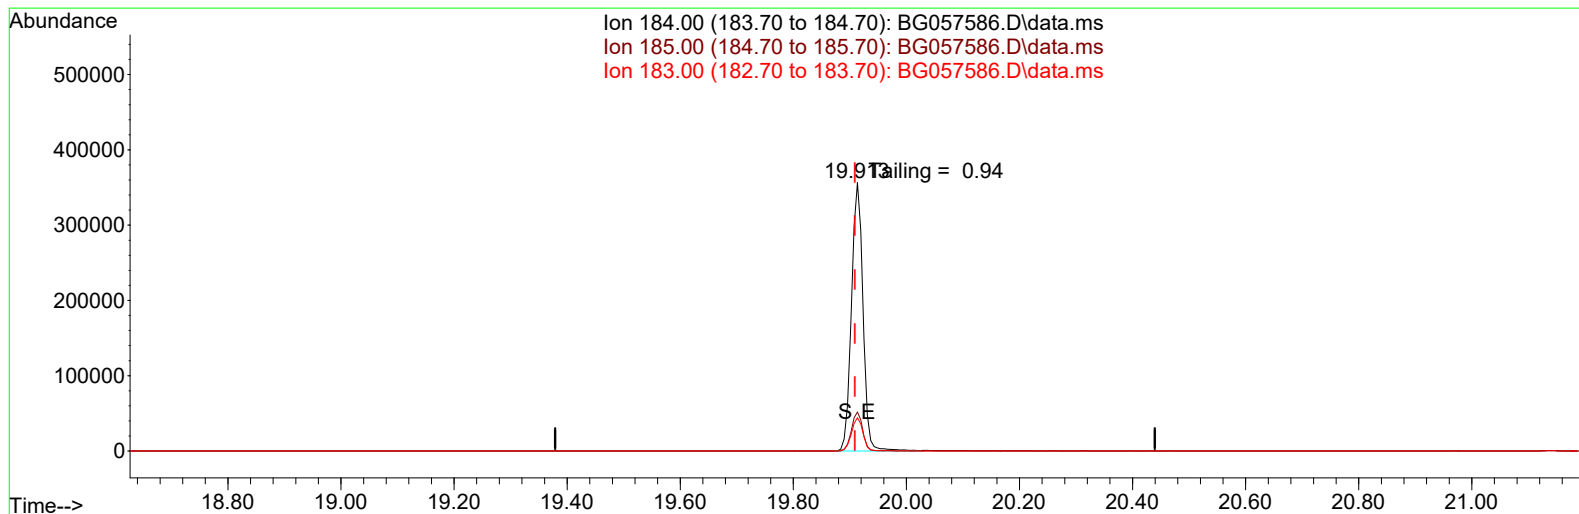

TIC: BG057586.D\data.ms

(77) Benzidine

19.913min (+ 0.004) 0.00 ng

response 505296

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.58
183.00	12.50	12.43
0.00	0.00	0.00