


Data Path : Z:\HPCHEM1\BNA_G\Data\BG052815\
 Data File : BG017320.D
 Acq On : 28 May 2015 12:02
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 28 04:22:03 2015

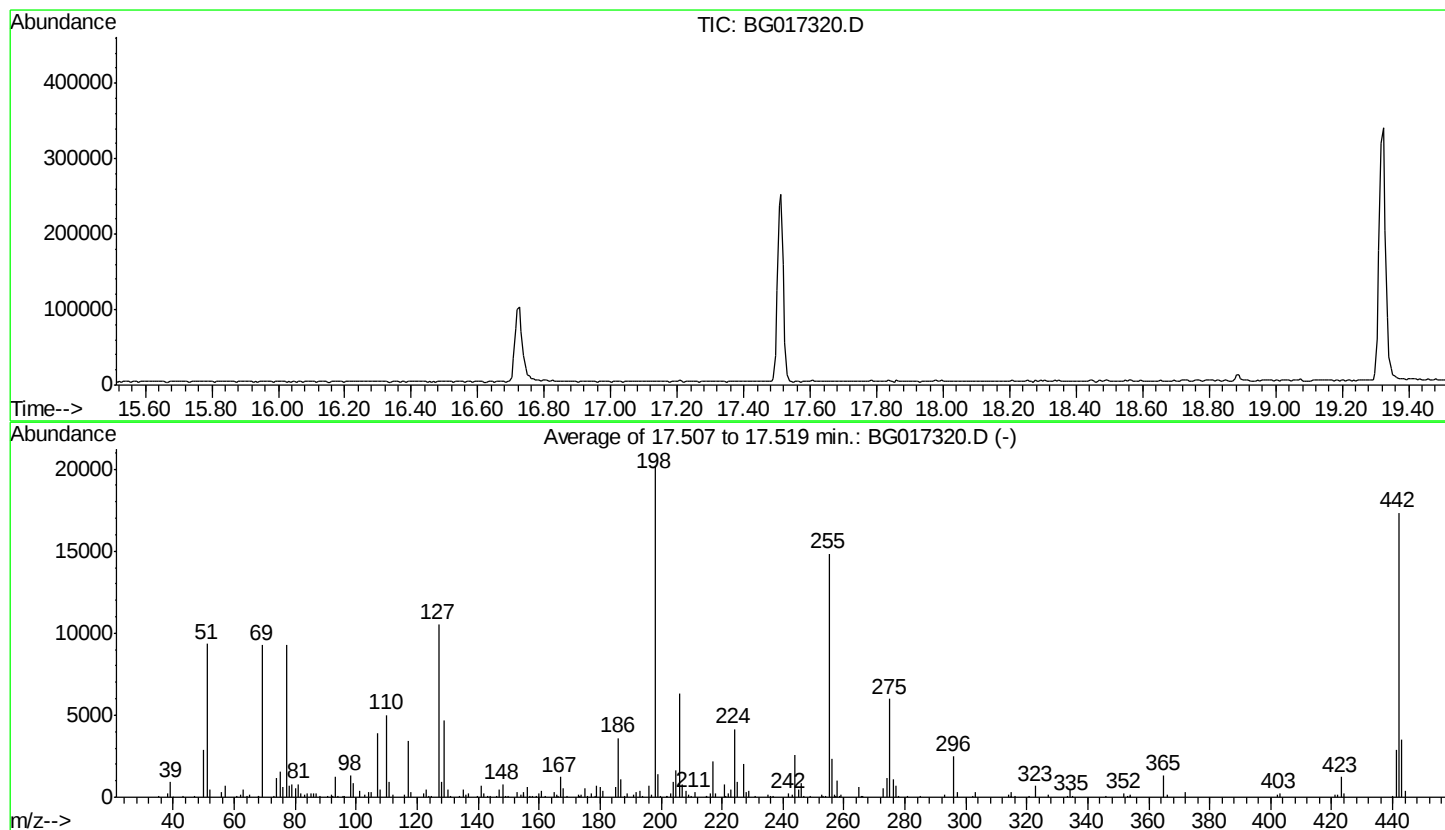

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	9340	PASS
68	69	0.00	2	0.7	67	PASS
69	198	0.00	100	45.9	9278	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.1	10516	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20201	PASS
199	198	5	9	7.1	1438	PASS
275	198	10	60	29.6	5972	PASS
365	198	1	100	6.4	1302	PASS
441	442	0.01	24	16.8	2909	PASS
442	198	50	100	85.8	17325	PASS
443	442	15	24	20.1	3482	PASS