


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052815\
 Data File : BG017338.D
 Acq On : 29 May 2015 00:35
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 28 04:22:03 2015

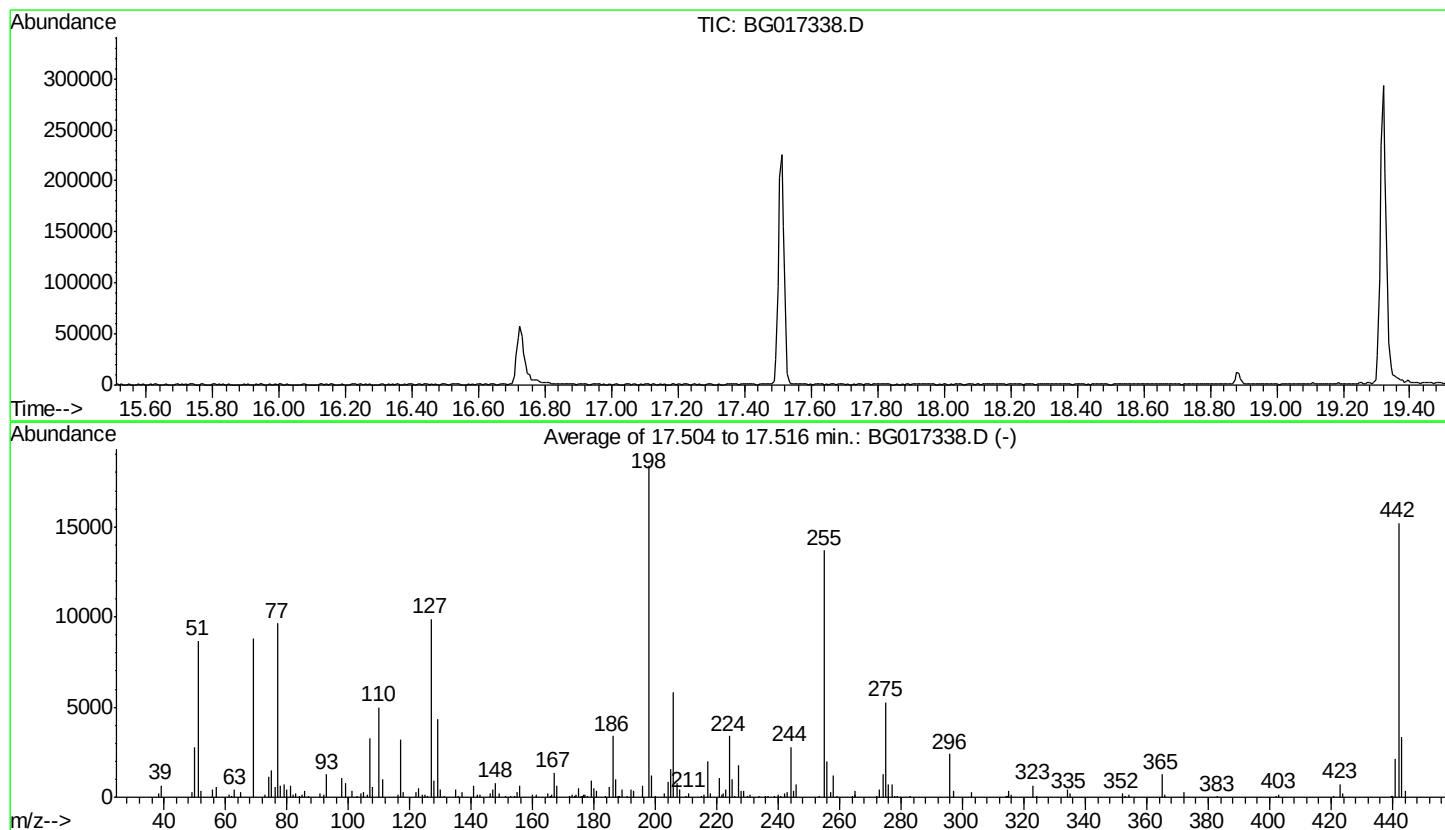

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	8675	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.0	8818	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.7	9876	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18389	PASS
199	198	5	9	6.7	1236	PASS
275	198	10	60	28.8	5287	PASS
365	198	1	100	6.9	1275	PASS
441	442	0.01	24	14.2	2161	PASS
442	198	50	100	82.6	15193	PASS
443	442	15	24	22.0	3339	PASS