
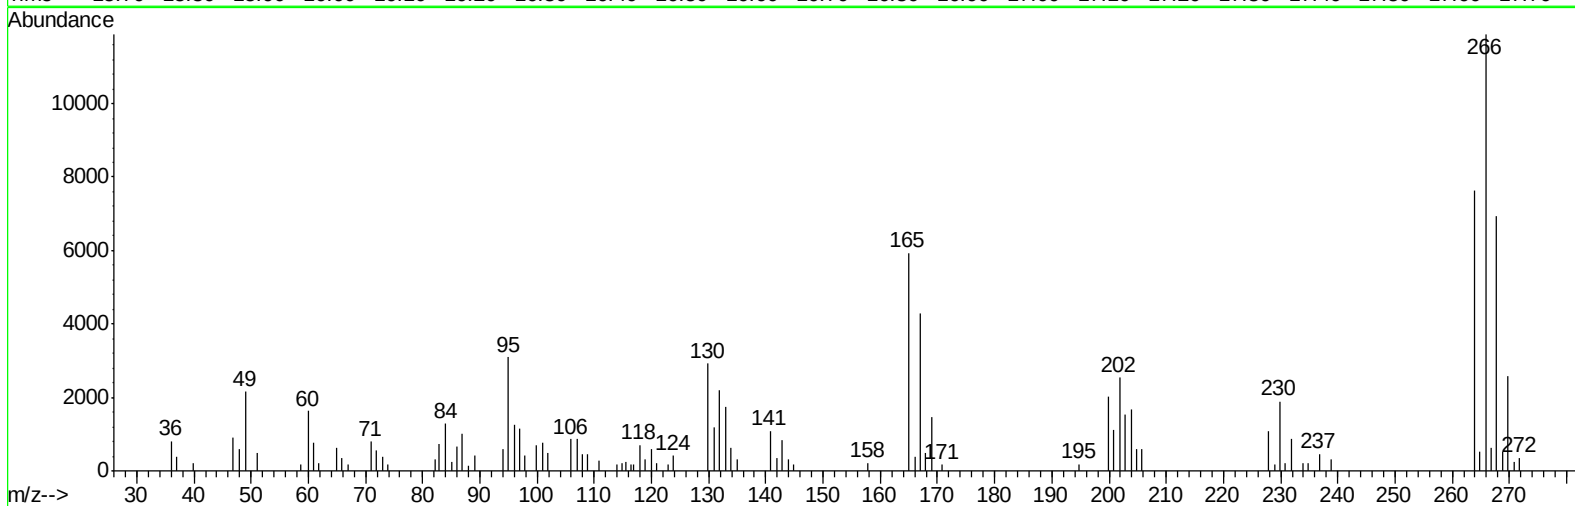


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052815\
Data File : BG017320.D
Acq On : 28 May 2015 12:02
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 05:08:31 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 29 03:19:24 2015
Response via : Initial Calibration

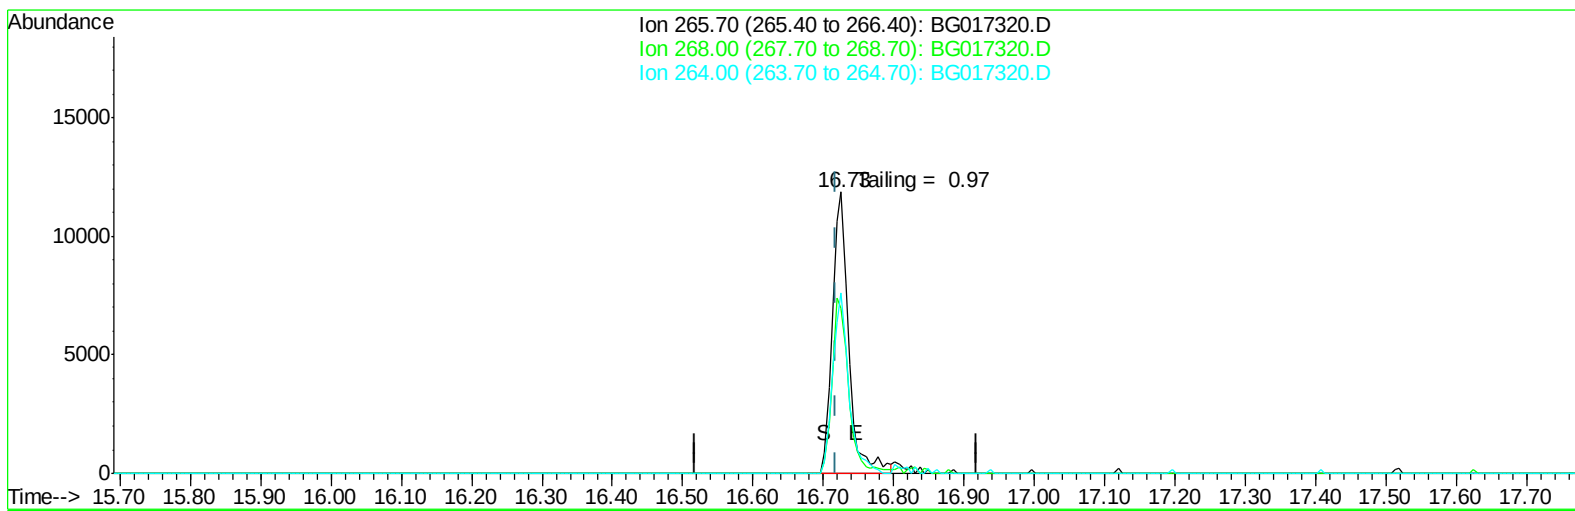

TIC: BG017320.D

(69) Pentachlorophenol (C)



16.725min (+0.007) 0.00ng

response 18367

Ion	Exp%	Act%
265.70	100	100
268.00	70.70	58.46
264.00	61.70	64.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052815\
Data File : BG017320.D
Acq On : 28 May 2015 12:02
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 05:08:31 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 29 03:19:24 2015
Response via : Initial Calibration

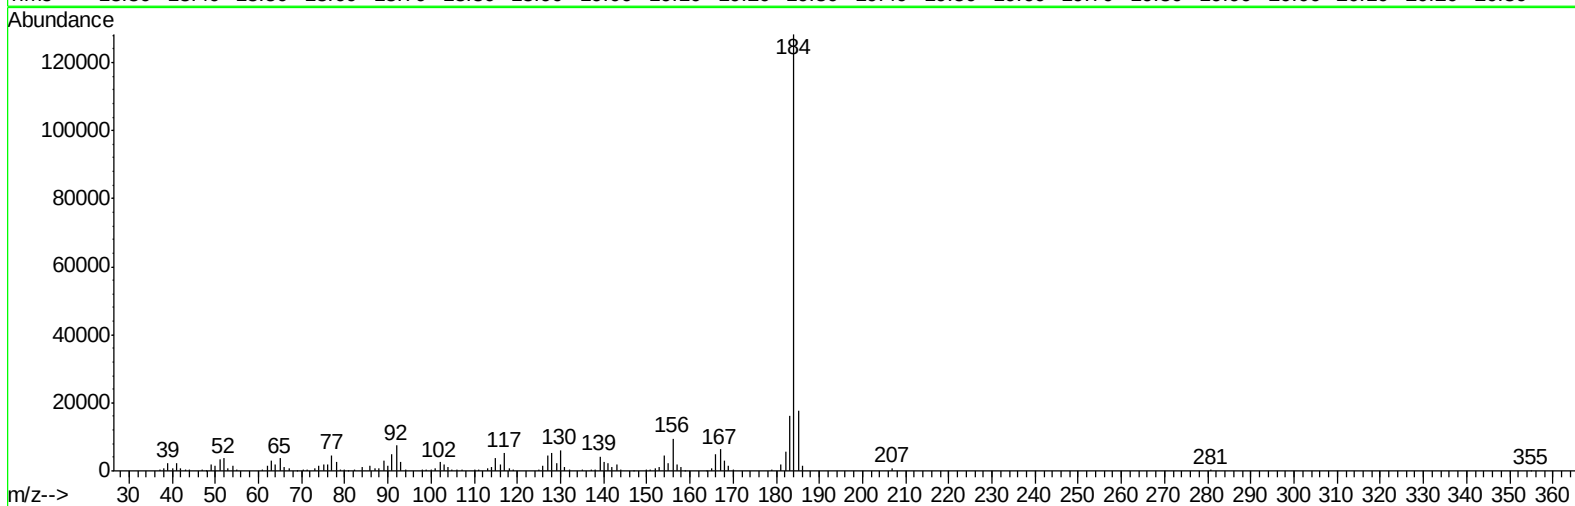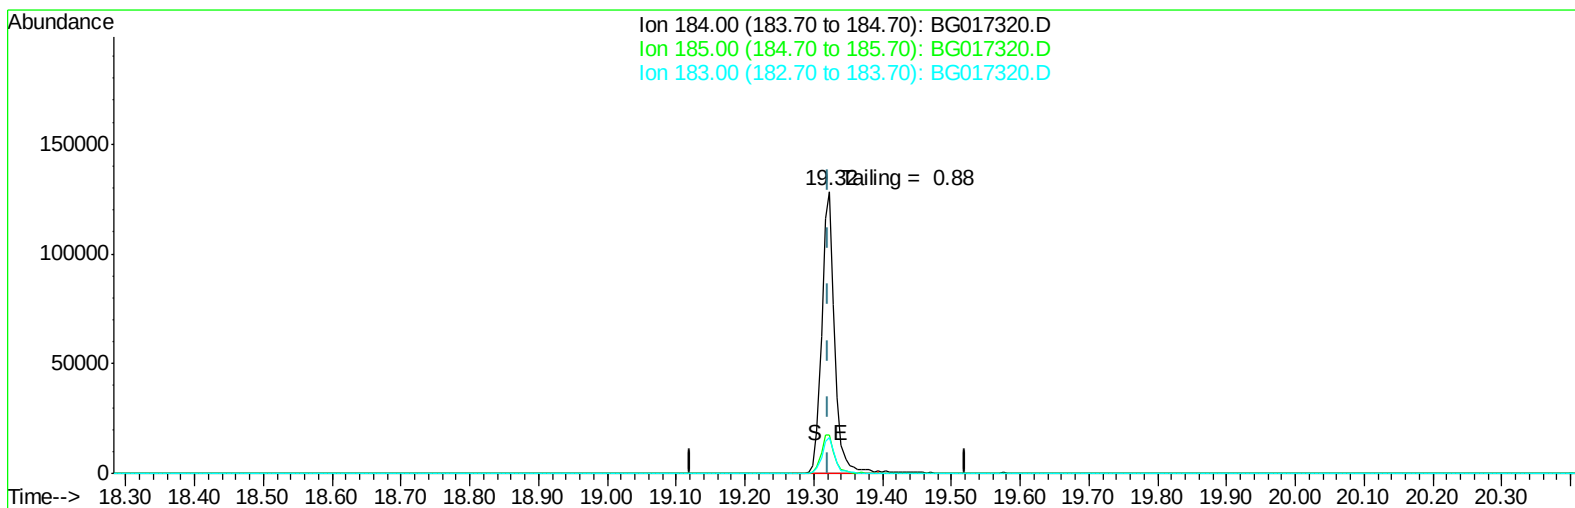

TIC: BG017320.D

(76) Benzidine

19.322min (+0.001) 0.00ng

response 168365

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	13.75
183.00	14.30	12.66
0.00	0.00	0.00