


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052815\
Data File : BG017338.D
Acq On : 29 May 2015 00:35
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 05:09:29 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 29 03:19:24 2015
Response via : Initial Calibration

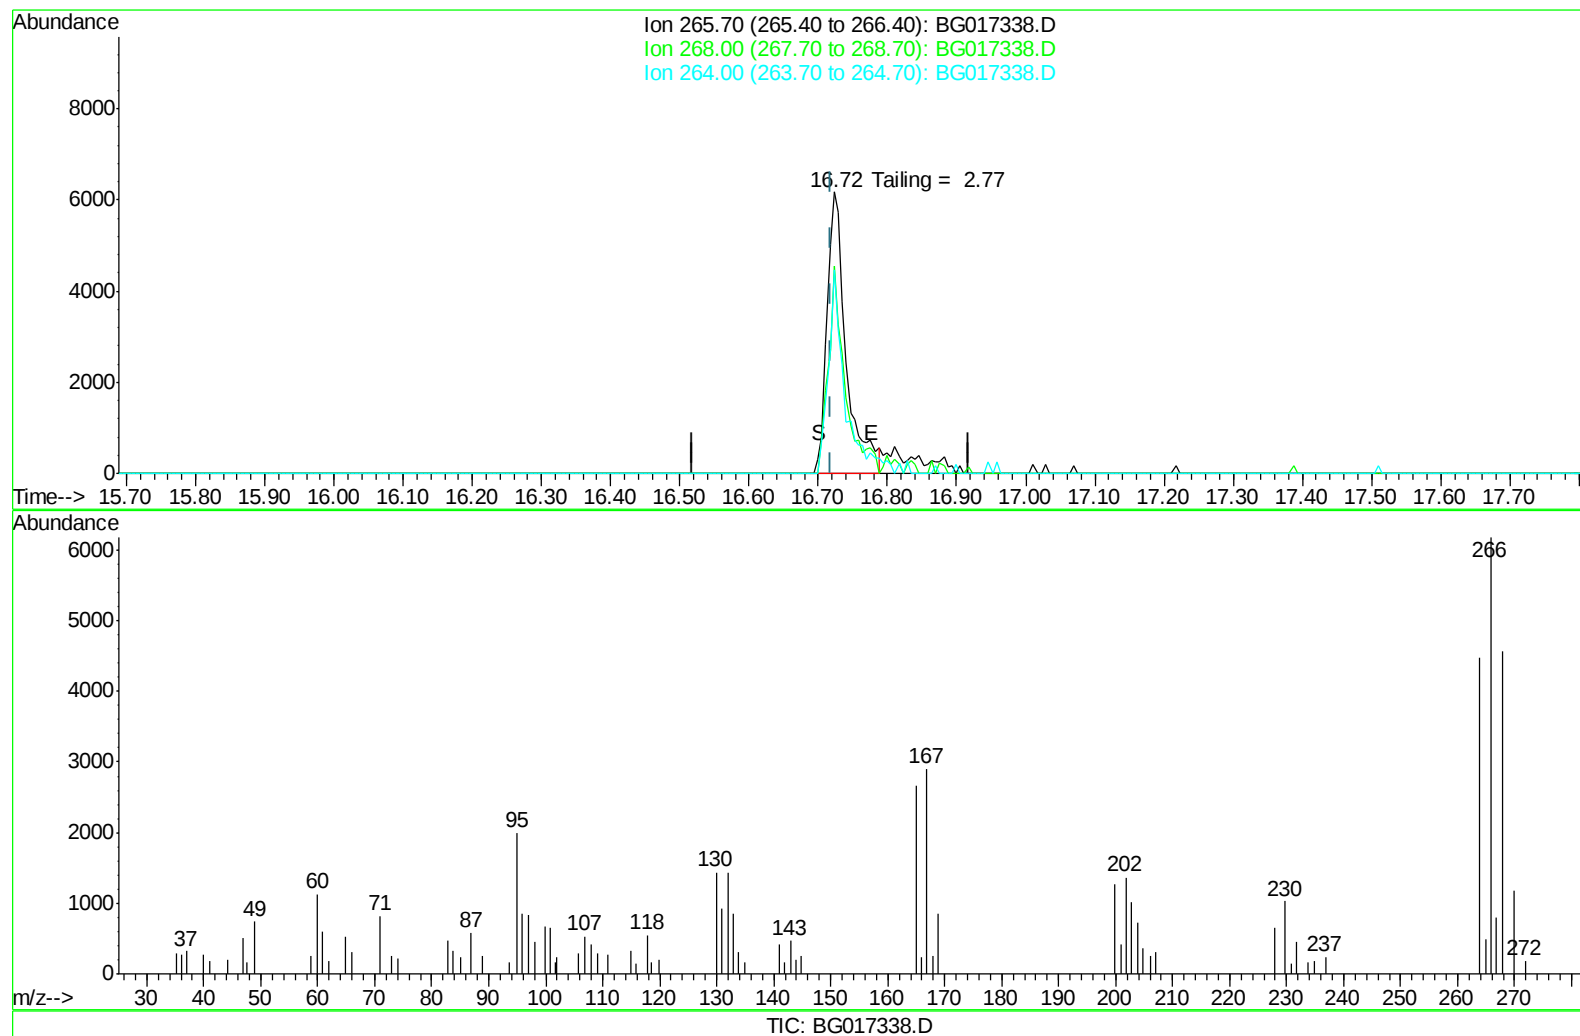

(69) Pentachlorophenol (C)



16.723min (+0.004) 0.00ng m

response 11829

Ion	Exp%	Act%
265.70	100	100
268.00	70.70	73.87
264.00	61.70	72.44
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG052815\
Data File : BG017338.D
Acq On : 29 May 2015 00:35
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 05:09:29 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 29 03:19:24 2015
Response via : Initial Calibration

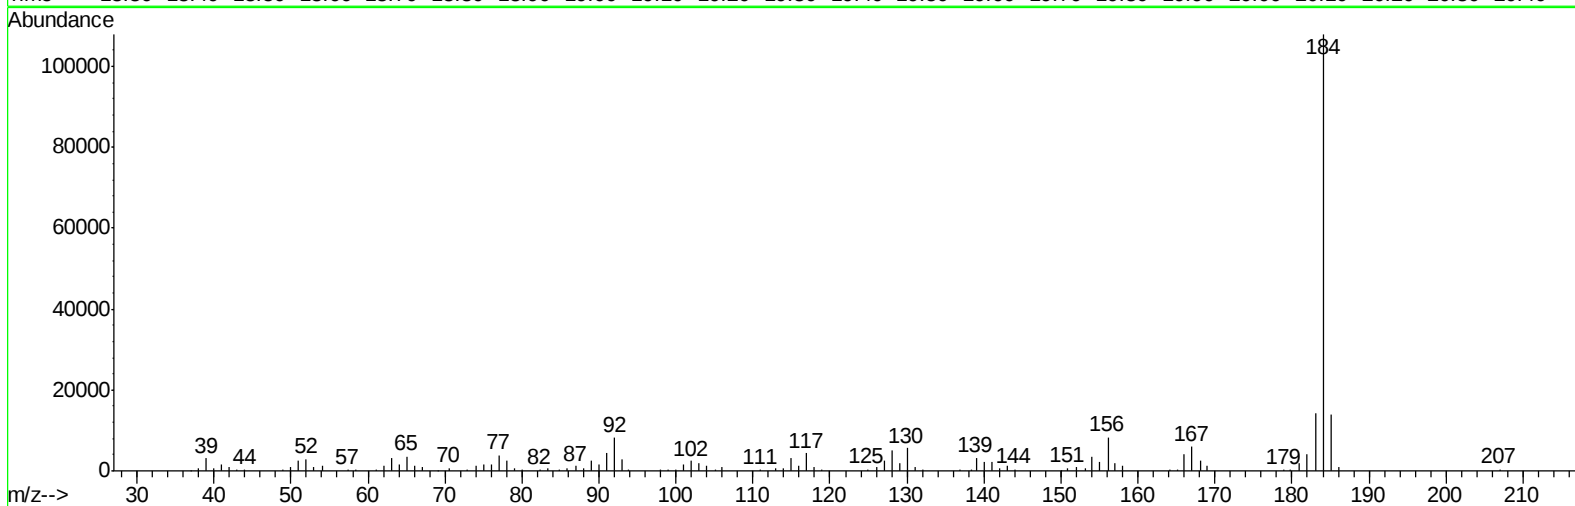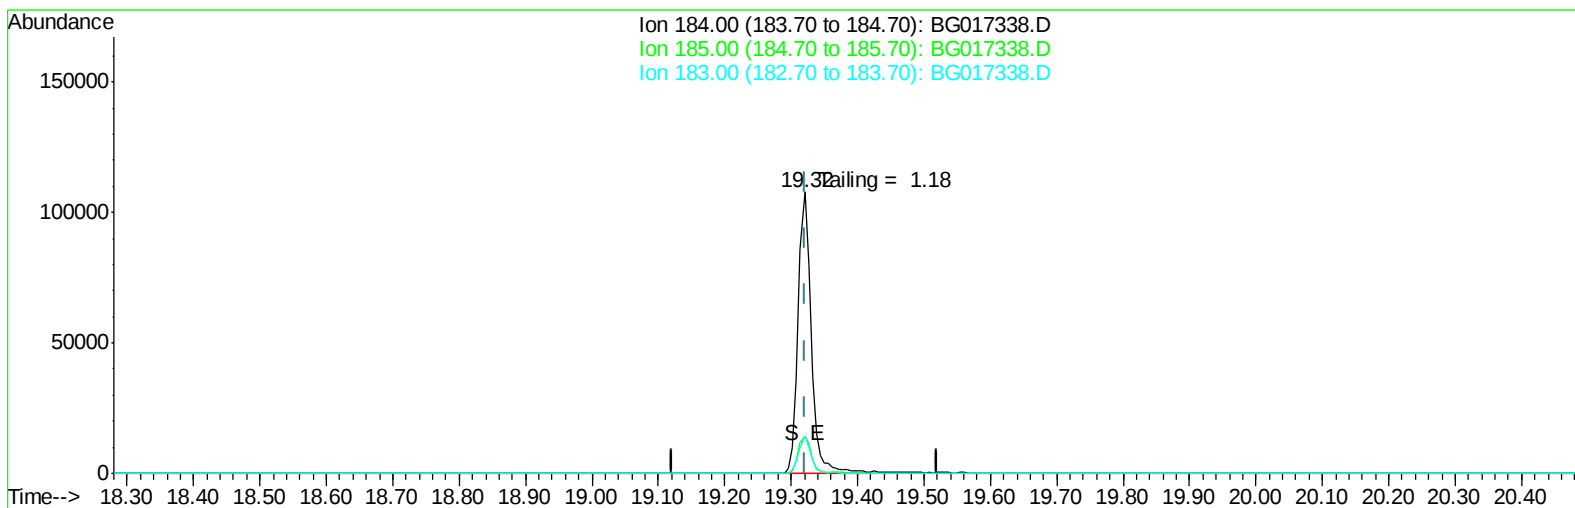

TIC: BG017338.D

(76) Benzidine

19.320min (-0.001) 0.00ng

response 143754

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	13.00
183.00	14.30	13.18
0.00	0.00	0.00