


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG052820\
 Data File : BG045491.D
 Acq On : 28 May 2020 10:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 07:27:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 28 13:15:42 2020
 Response via : Initial Calibration

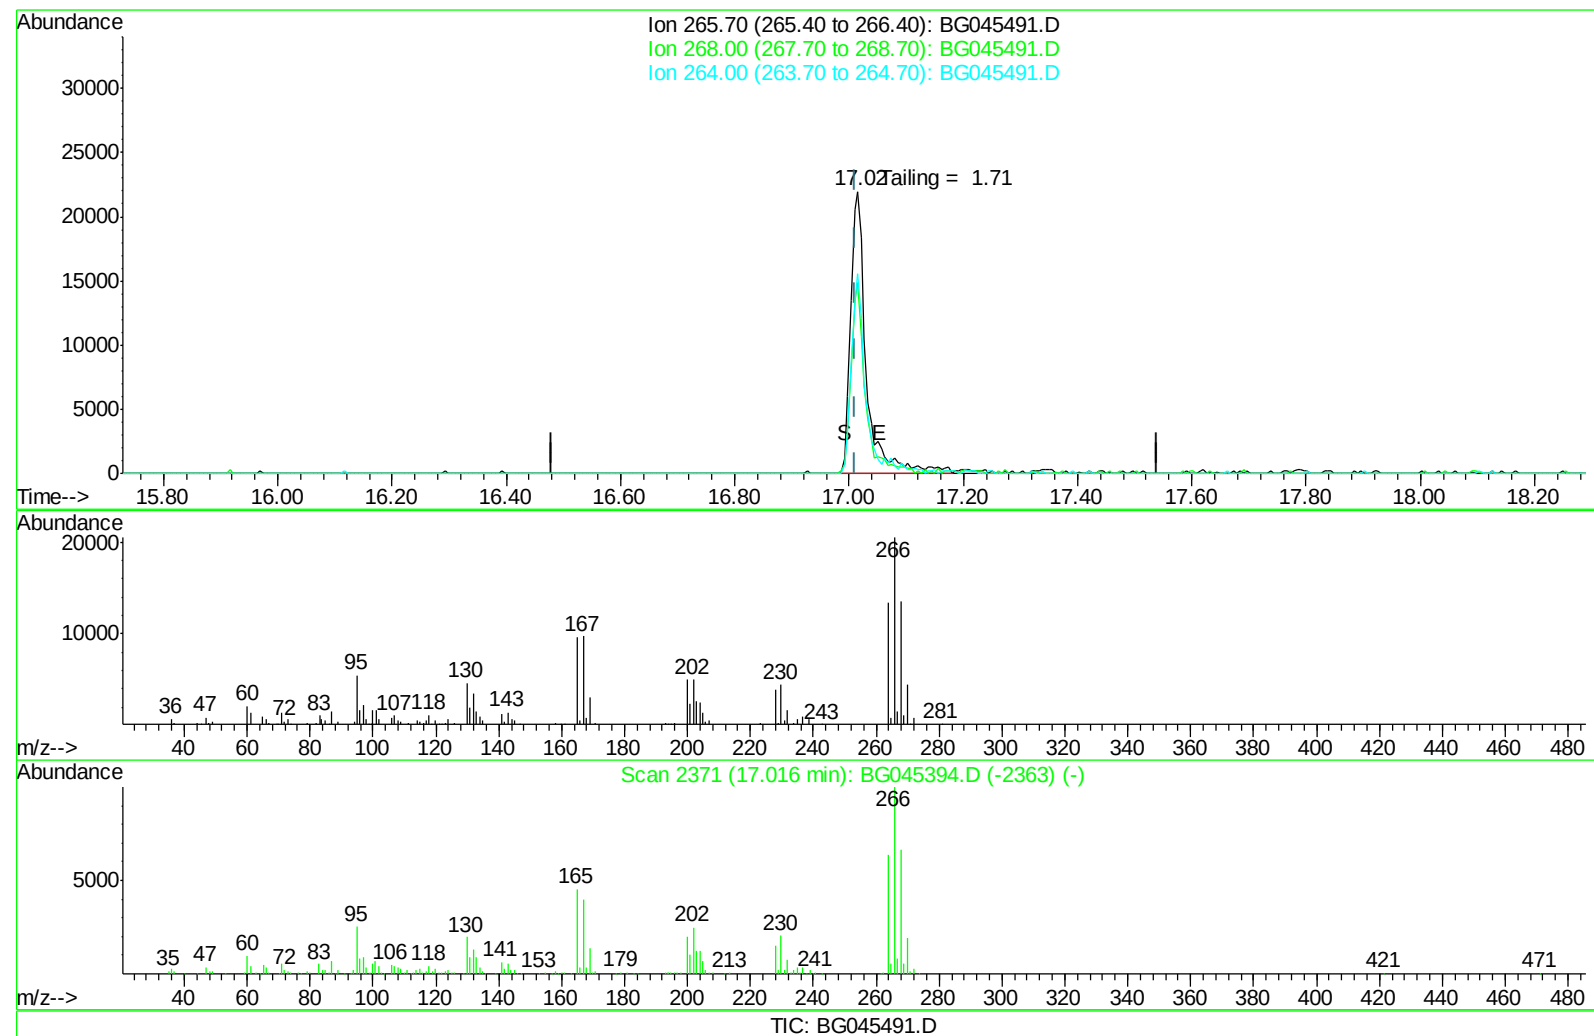

(70) Pentachlorophenol (C)




17.015min (+0.004) 15944.97ng

response 39101

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	67.58
264.00	63.70	70.97
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG052820\
 Data File : BG045491.D
 Acq On : 28 May 2020 10:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 07:27:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 28 13:15:42 2020
 Response via : Initial Calibration

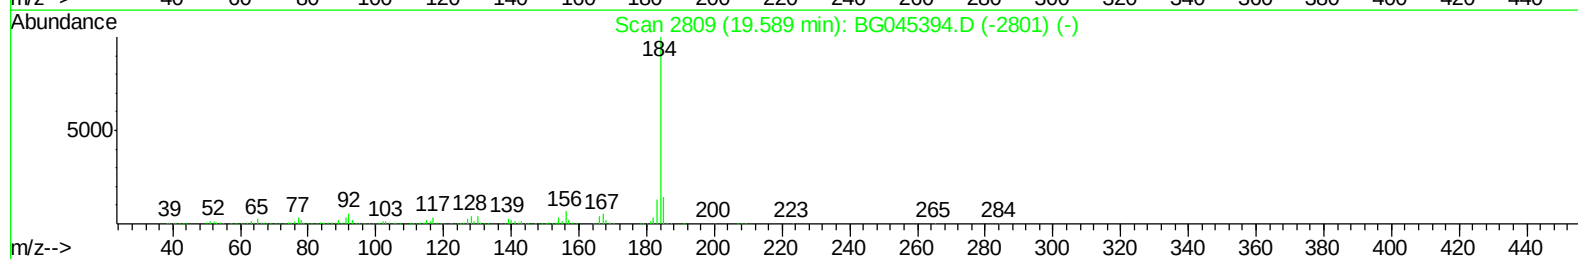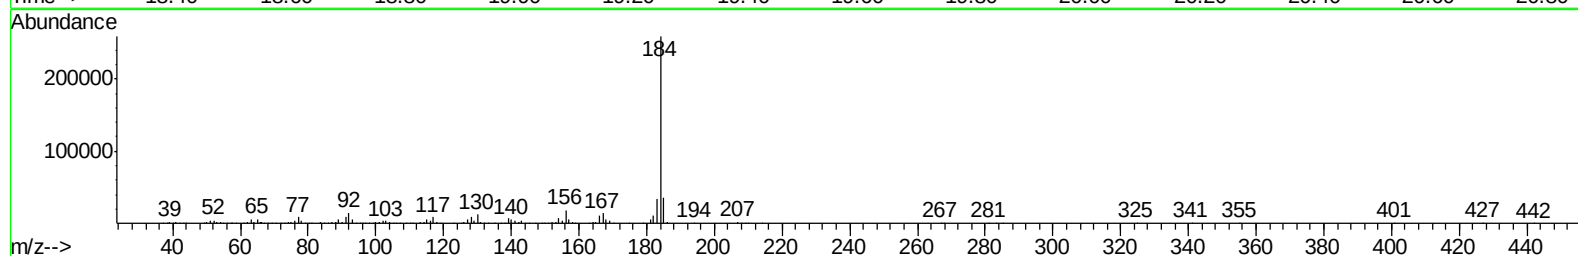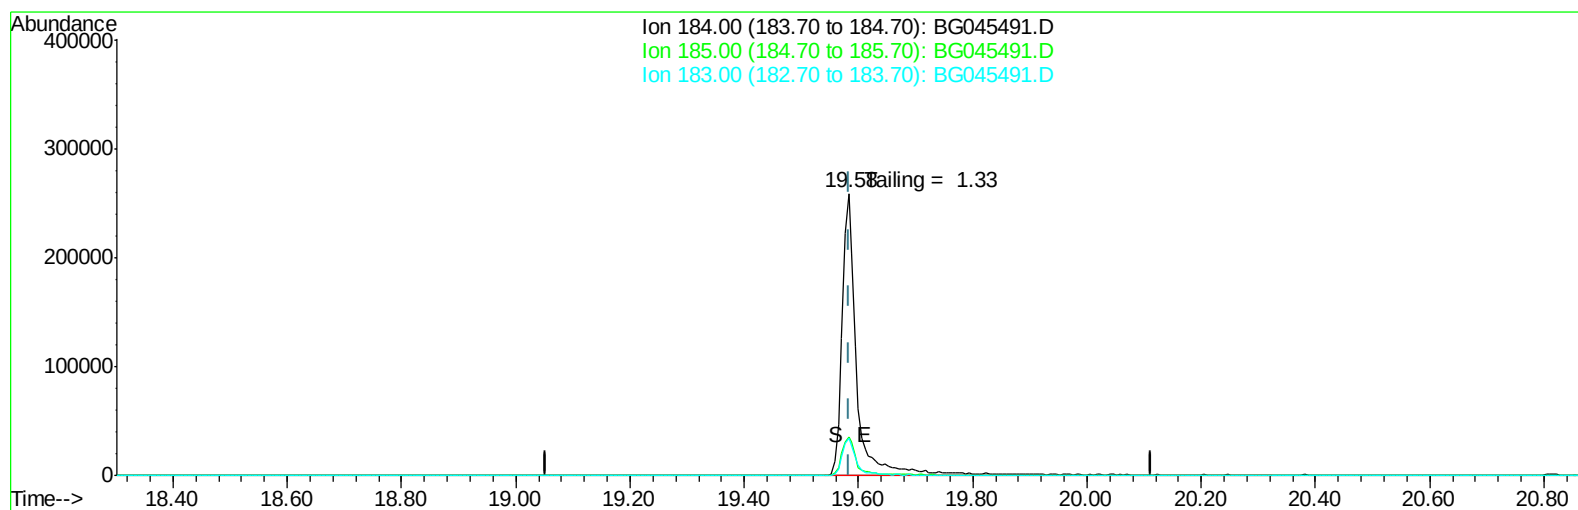

TIC: BG045491.D

(77) Benzidine

19.582min (-0.002) 261610.00ng

response 396762

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	13.72
183.00	12.80	13.06
0.00	0.00	0.00