
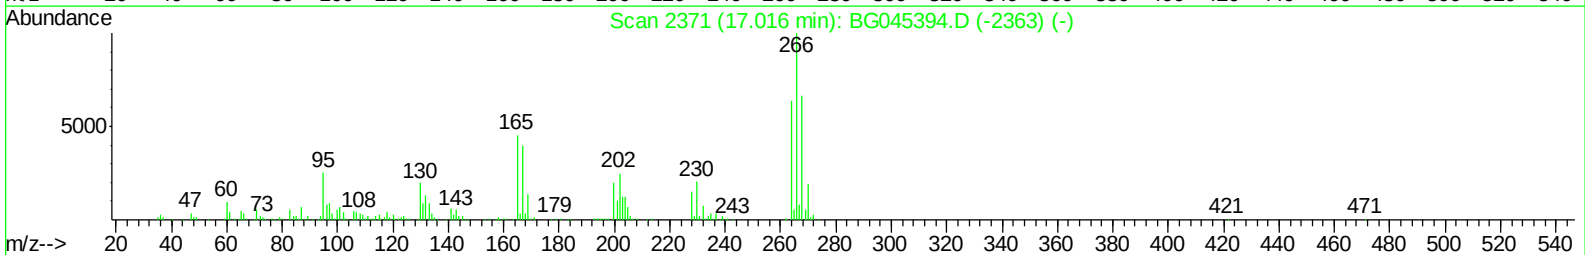
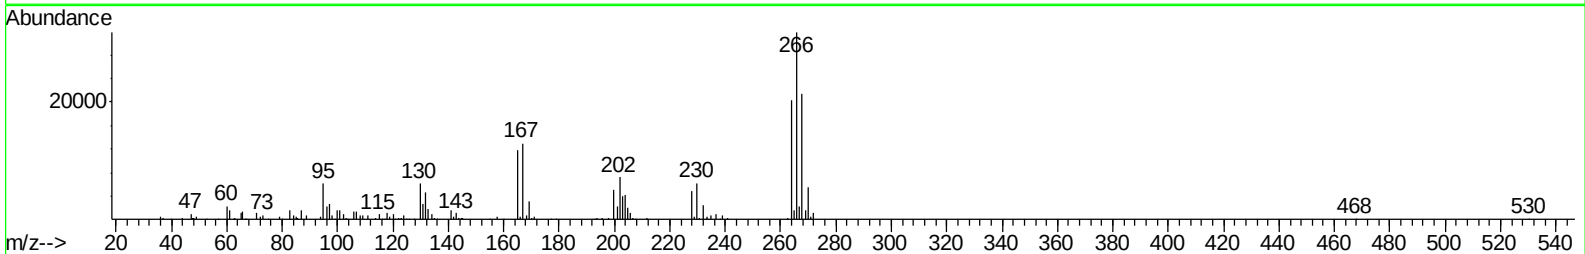


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG052820\  
Data File : BG045508.D  
Acq On : 29 May 2020 00:22  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 01:01:40 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu May 28 13:15:42 2020  
Response via : Initial Calibration

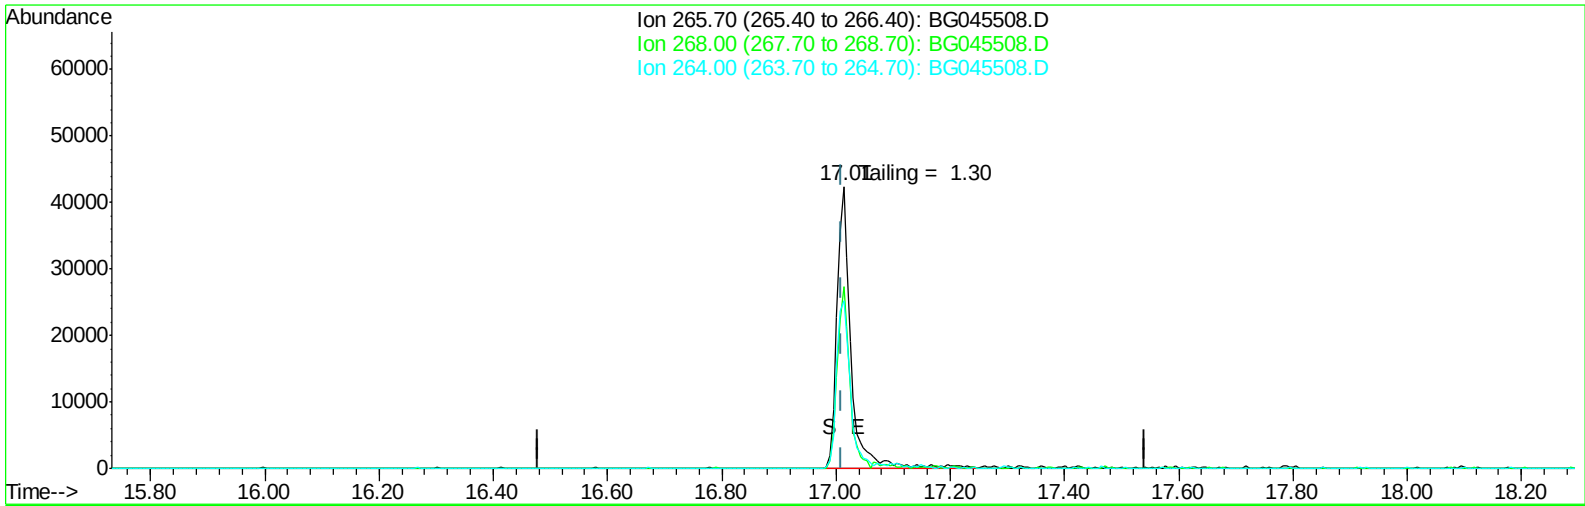

TIC: BG045508.D

(70) Pentachlorophenol (C)




17.013min (+0.002) 37937.40ng

response 68268

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 66.50 | 64.49 |
| 264.00 | 63.70 | 59.74 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG052820\  
 Data File : BG045508.D  
 Acq On : 29 May 2020 00:22  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 01:01:40 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu May 28 13:15:42 2020  
 Response via : Initial Calibration

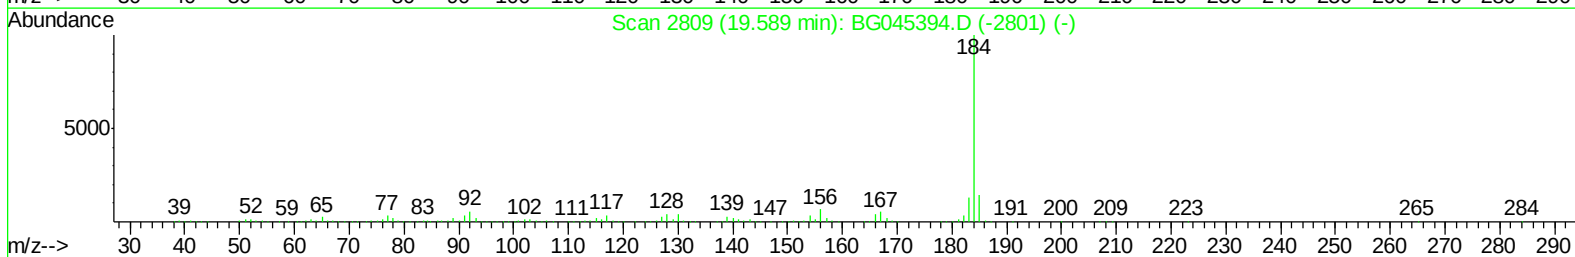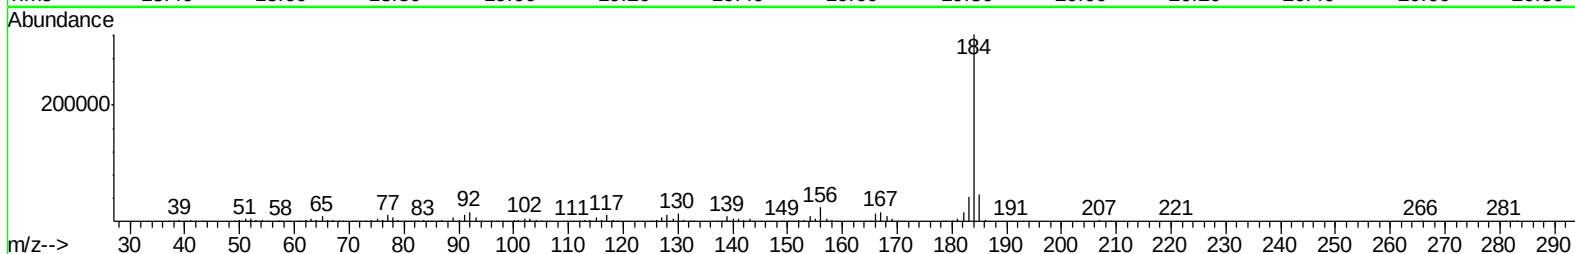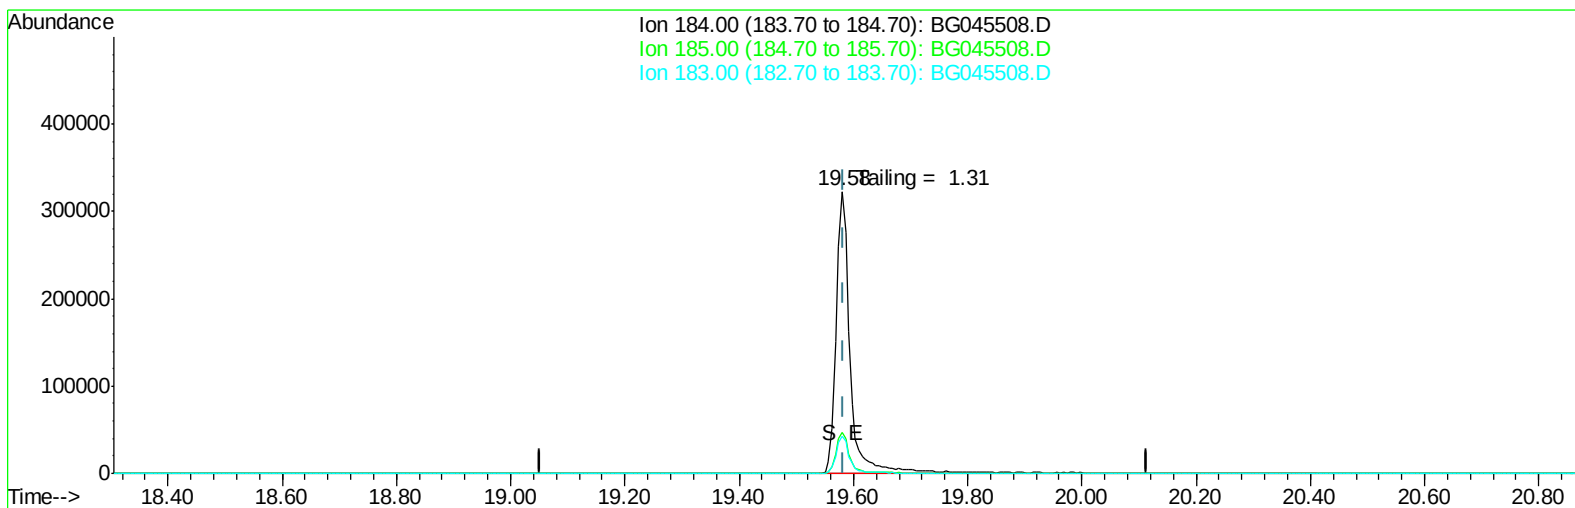

TIC: BG045508.D

(77) Benzidine

19.580min (-0.004) 331738.39ng

response 540388

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.60 | 14.75 |
| 183.00 | 12.80 | 13.02 |
| 0.00   | 0.00  | 0.00  |