


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG052820\
 Data File : BG045491.D
 Acq On : 28 May 2020 10:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 28 13:15:42 2020

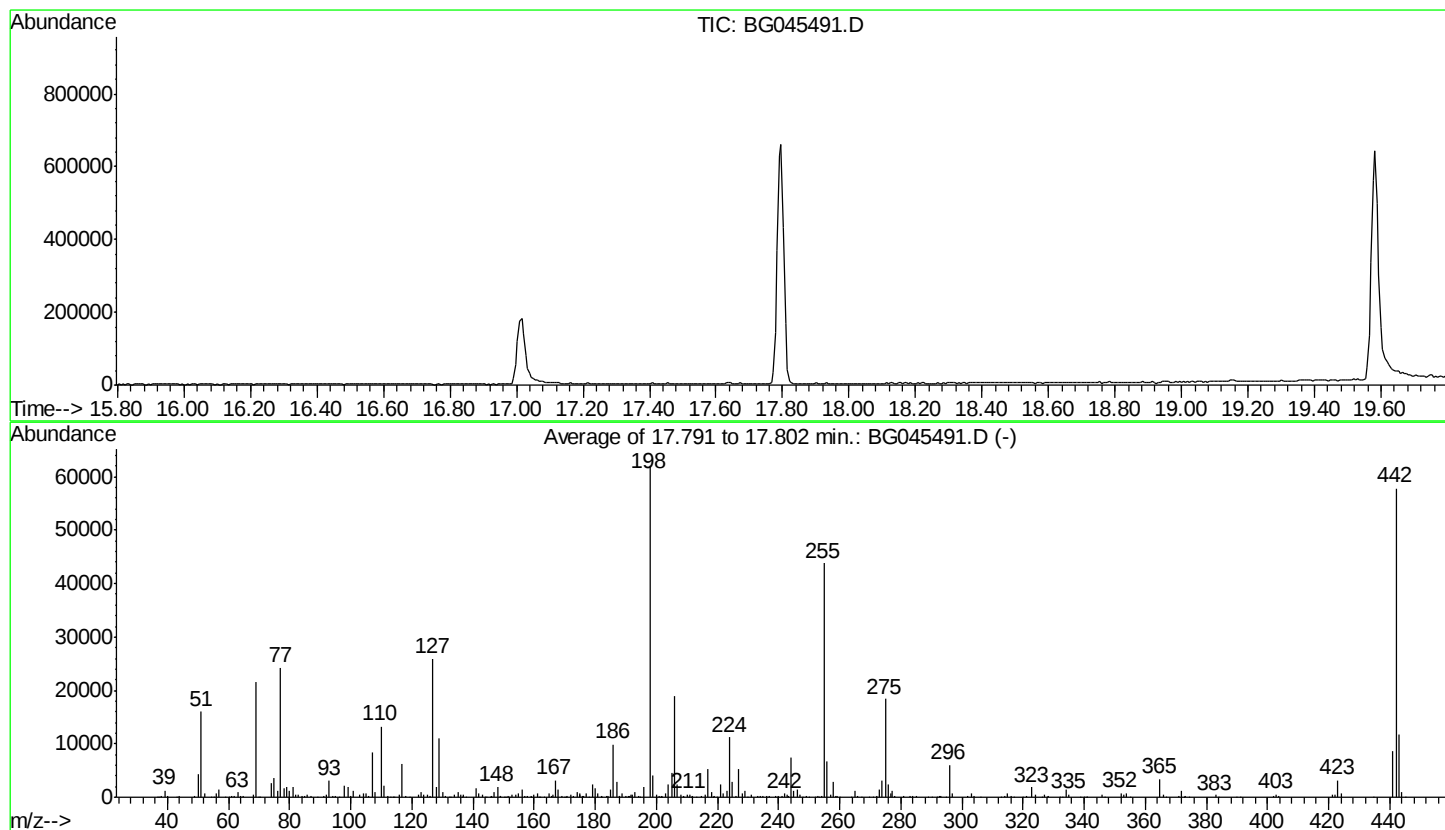

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	16016	PASS
68	69	0.00	2	1.7	371	PASS
69	198	0.00	100	34.8	21635	PASS
70	69	0.00	2	0.3	75	PASS
127	198	10	80	41.8	25938	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62085	PASS
199	198	5	9	6.7	4147	PASS
275	198	10	60	29.7	18445	PASS
365	198	1	100	5.6	3479	PASS
441	198	0.01	100	14.0	8704	PASS
442	198	50	100	93.2	57874	PASS
443	442	15	24	20.2	11663	PASS