


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG052820\
 Data File : BG045508.D
 Acq On : 29 May 2020 00:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 28 13:15:42 2020

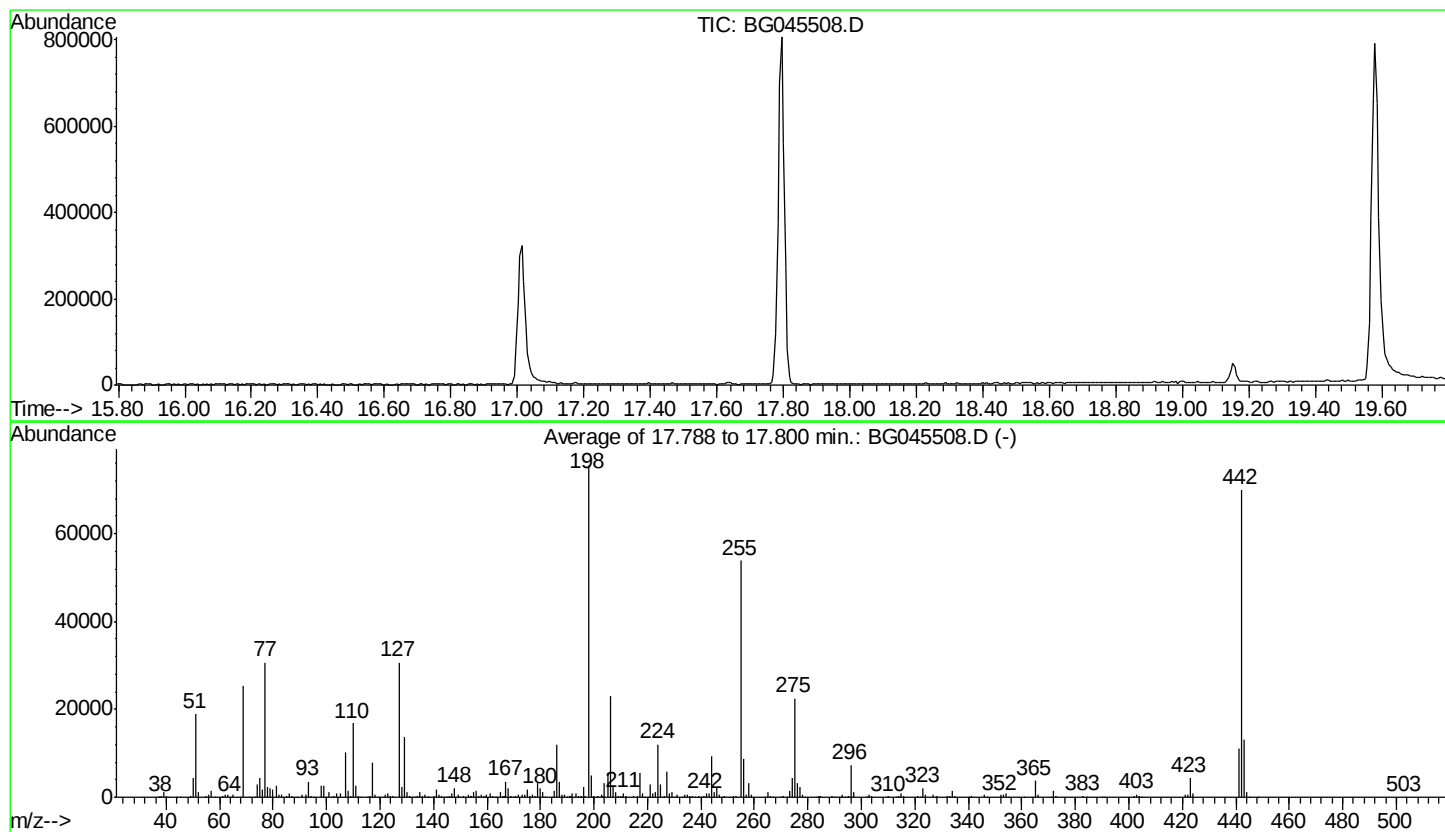

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	19072	PASS
68	69	0.00	2	0.4	94	PASS
69	198	0.00	100	33.6	25338	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.6	30616	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75469	PASS
199	198	5	9	6.6	4964	PASS
275	198	10	60	29.9	22584	PASS
365	198	1	100	4.9	3691	PASS
441	198	0.01	100	14.6	11028	PASS
442	198	50	100	92.7	69930	PASS
443	442	15	24	18.8	13174	PASS