
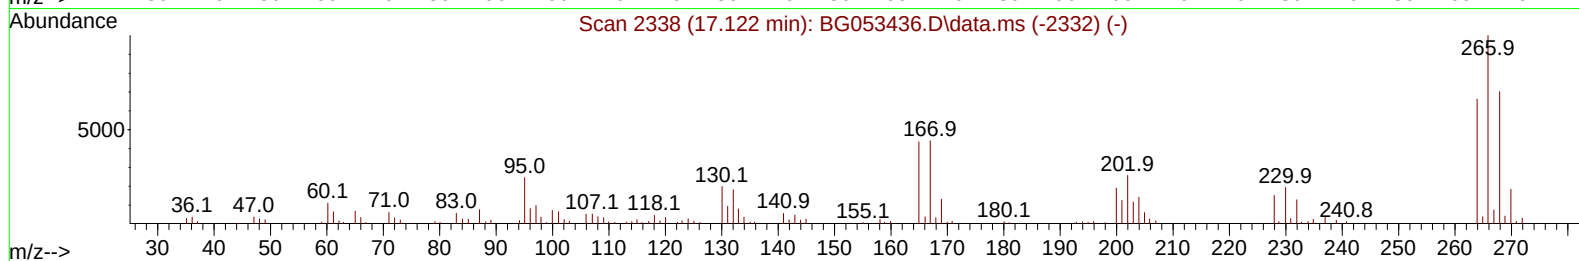
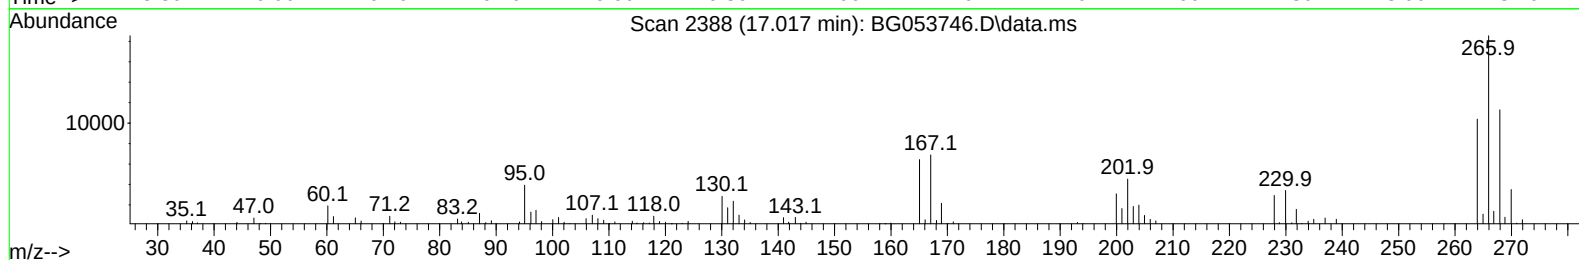


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053746.D
Acq On : 28 May 2022 10:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 11:04:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

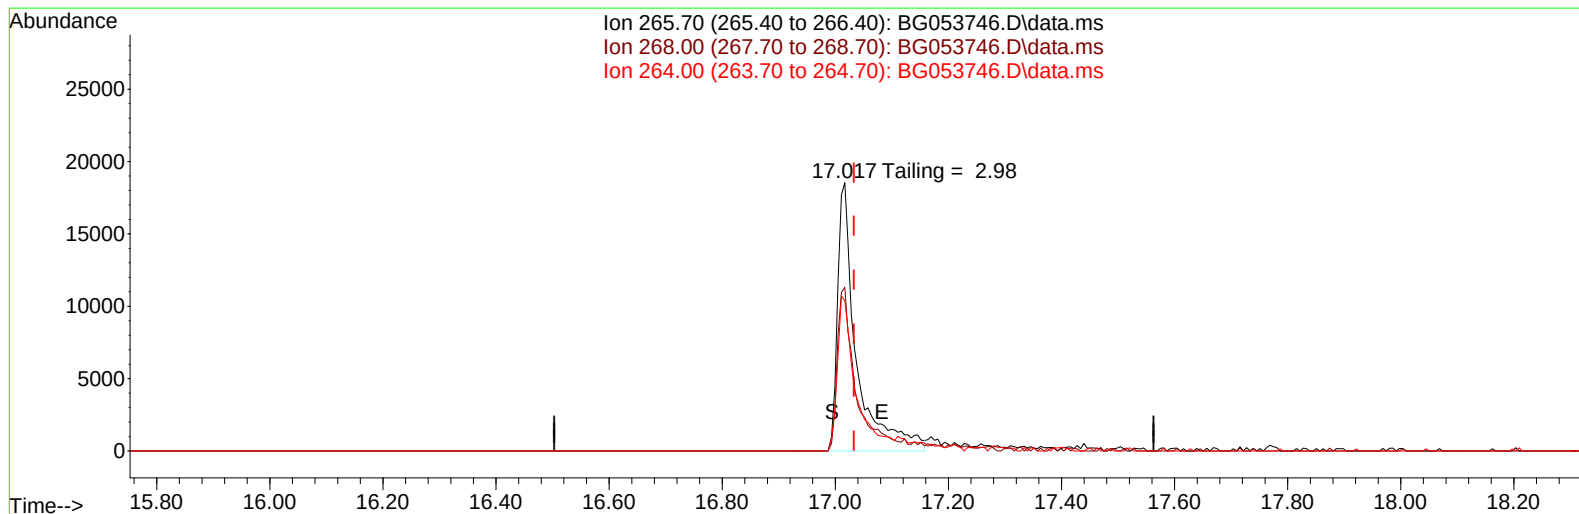

TIC: BG053746.D\data.ms

(70) Pentachlorophenol (C)




17.017min (-0.016) 27167.97 ng

response 42114

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	60.95
264.00	66.20	56.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053746.D
Acq On : 28 May 2022 10:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 11:04:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

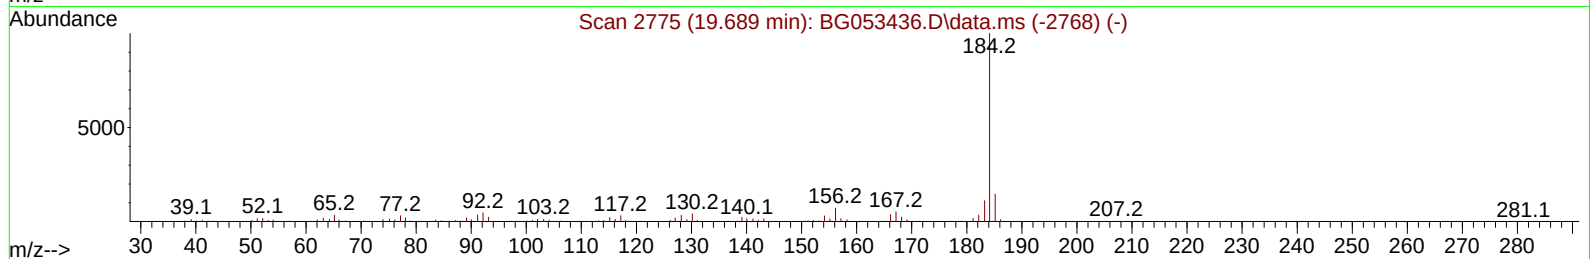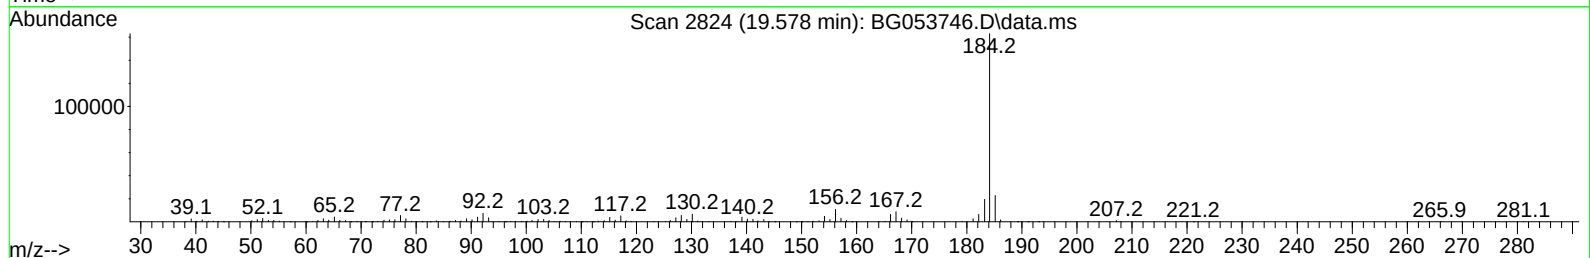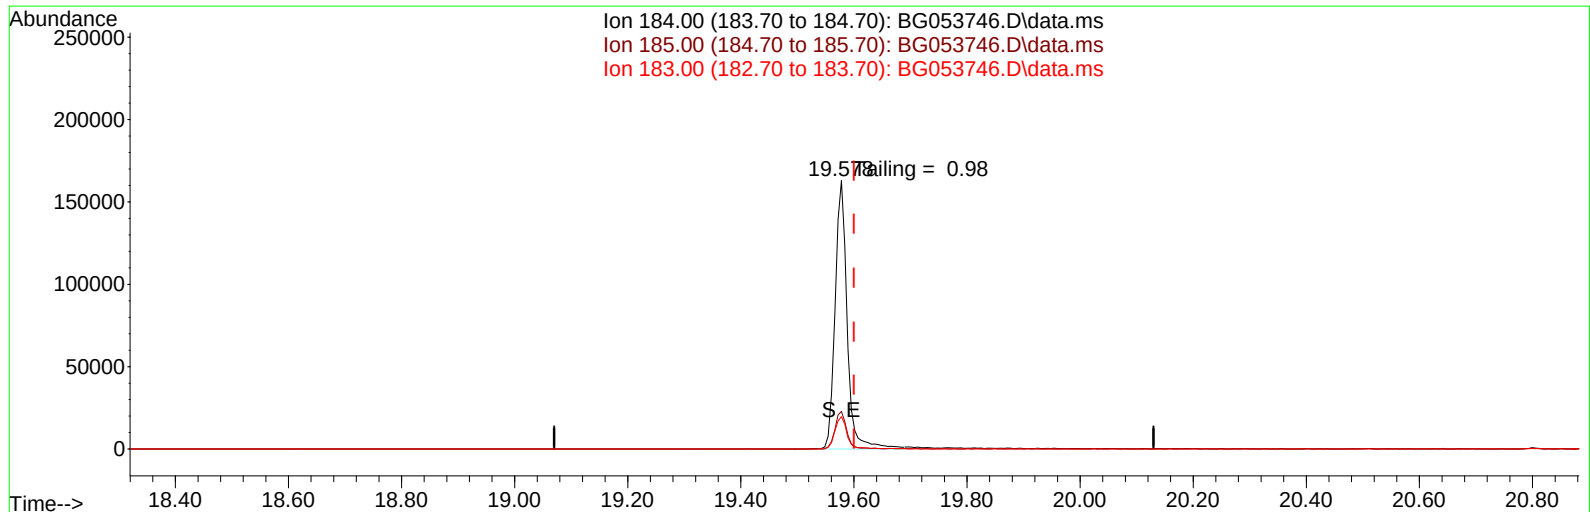

TIC: BG053746.D\data.ms

(77) Benzidine**19.578min (-0.022) 5616.57 ng****response 242842**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.01
183.00	11.10	12.04
0.00	0.00	0.00