

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
 Data File : BG053748.D
 Acq On : 28 May 2022 13:09
 Operator : CG/JU
 Sample : PB145086BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB145086BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053748.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	4	8	15	rVB	17139	22589	1.12%	0.330%
2	5.525	426	432	447	rBV	330364	546183	27.01%	7.971%
3	7.146	702	708	722	rBV	345676	620748	30.69%	9.059%
4	7.951	835	845	853	rBV	57038	96876	4.79%	1.414%
5	9.114	1035	1043	1056	rBV	221779	403297	19.94%	5.885%
6	10.759	1317	1323	1335	rVB	75866	135025	6.68%	1.970%
7	13.214	1734	1741	1752	rBV	645445	989946	48.95%	14.447%
8	14.595	1968	1976	1983	rBV	141962	215393	10.65%	3.143%
9	16.087	2224	2230	2241	rBV	489201	802938	39.70%	11.717%
10	17.338	2437	2443	2452	rBV	198482	304156	15.04%	4.439%
11	19.952	2882	2888	2901	rBV	1559454	2022476	100.00%	29.514%
12	21.603	3163	3169	3176	rBV	219004	357818	17.69%	5.222%
13	24.781	3701	3710	3720	rBV	120566	335045	16.57%	4.889%




Sum of corrected areas: 6852490

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053748.D
Acq On : 28 May 2022 13:09
Operator : CG/JU
Sample : PB145086BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145086BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

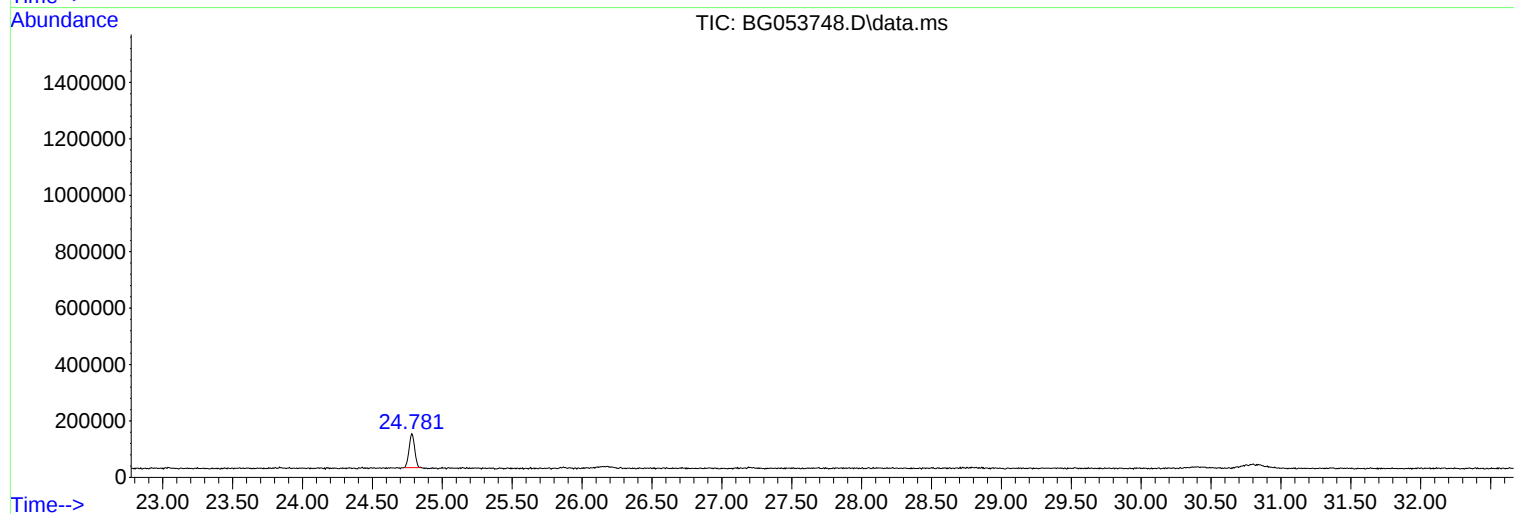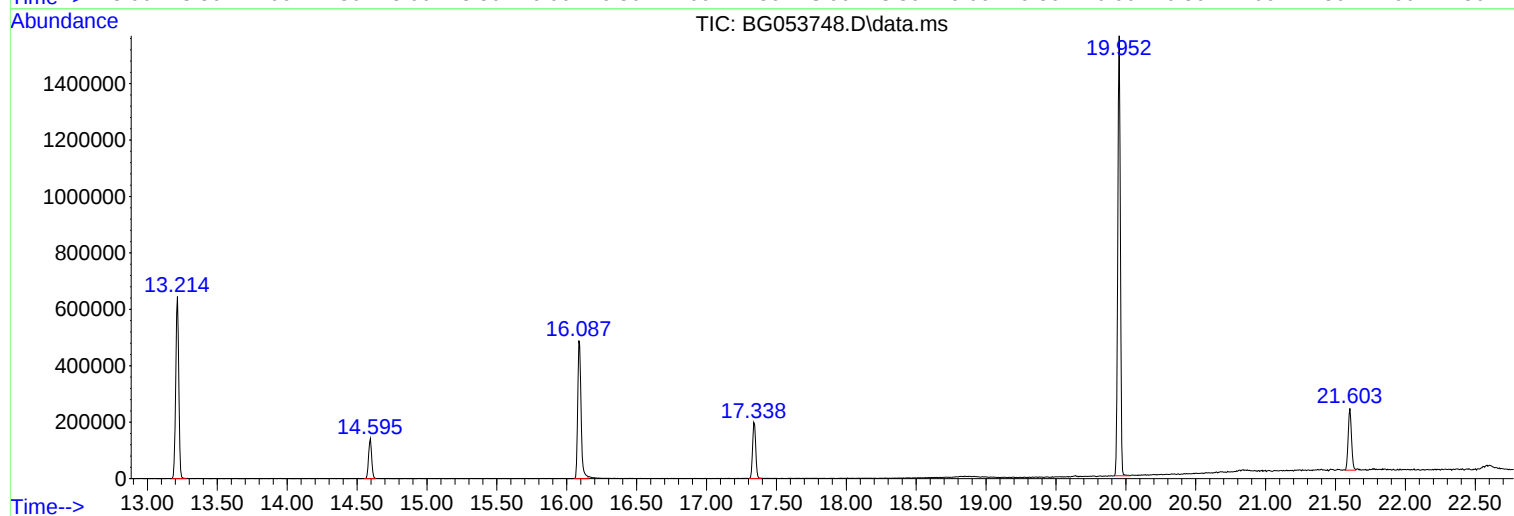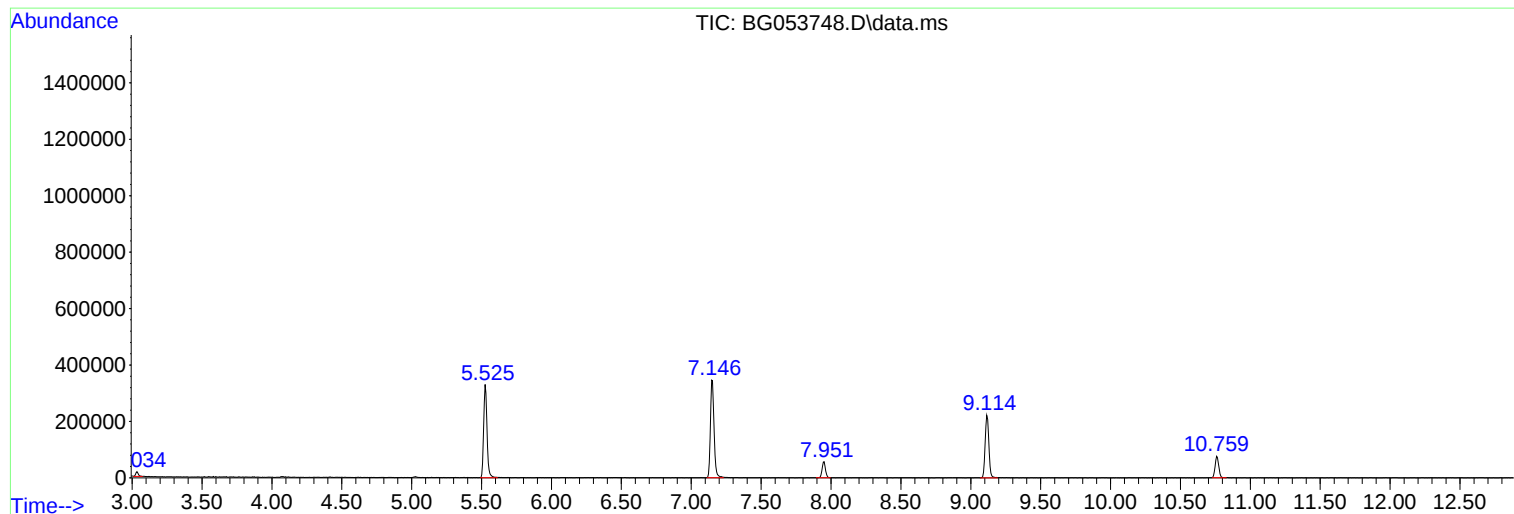

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053748.D
Acq On : 28 May 2022 13:09
Operator : CG/JU
Sample : PB145086BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145086BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053748.D
Acq On : 28 May 2022 13:09
Operator : CG/JU
Sample : PB145086BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145086BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------