

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
 Data File : BG053749.D
 Acq On : 28 May 2022 13:51
 Operator : CG/JU
 Sample : N3080-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC-5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053749.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.041	3	9	22	rVB	139750	252927	19.16%	3.484%
2	5.026	341	347	355	rVB2	11774	20958	1.59%	0.289%
3	5.532	426	433	446	rBV	397712	626259	47.43%	8.626%
4	7.147	700	708	721	rBV	309694	555108	42.04%	7.646%
5	7.946	837	844	852	rVB	78600	124565	9.43%	1.716%
6	9.115	1033	1043	1050	rBV	182138	324623	24.59%	4.471%
7	10.760	1314	1323	1332	rBV	98358	177003	13.41%	2.438%
8	13.209	1732	1740	1750	rBV	554926	826347	62.59%	11.382%
9	14.079	1875	1888	1890	rBV6	31050	81164	6.15%	1.118%
10	14.590	1969	1975	1982	rVB	153512	243976	18.48%	3.360%
11	16.088	2224	2230	2241	rBV	475859	746348	56.53%	10.280%
12	16.734	2330	2340	2341	rBV4	48602	94069	7.12%	1.296%
13	17.339	2437	2443	2448	rBV	203162	297824	22.56%	4.102%
14	18.232	2588	2595	2612	rVB2	123075	317101	24.02%	4.368%
15	19.395	2789	2793	2799	rBV	29283	43905	3.33%	0.605%
16	19.501	2805	2811	2832	rVB2	133913	362514	27.46%	4.993%
17	19.759	2851	2855	2860	rVB	20293	28414	2.15%	0.391%
18	19.947	2882	2887	2893	rBV	1022215	1320317	100.00%	18.186%
19	20.629	2997	3003	3010	rVB	82939	115497	8.75%	1.591%
20	21.240	3103	3107	3113	rBV3	32784	50323	3.81%	0.693%
21	21.598	3162	3168	3173	rBV2	201923	335391	25.40%	4.620%
22	24.776	3702	3709	3719	rVB2	115215	315556	23.90%	4.346%


Sum of corrected areas: 7260189

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053749.D
Acq On : 28 May 2022 13:51
Operator : CG/JU
Sample : N3080-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

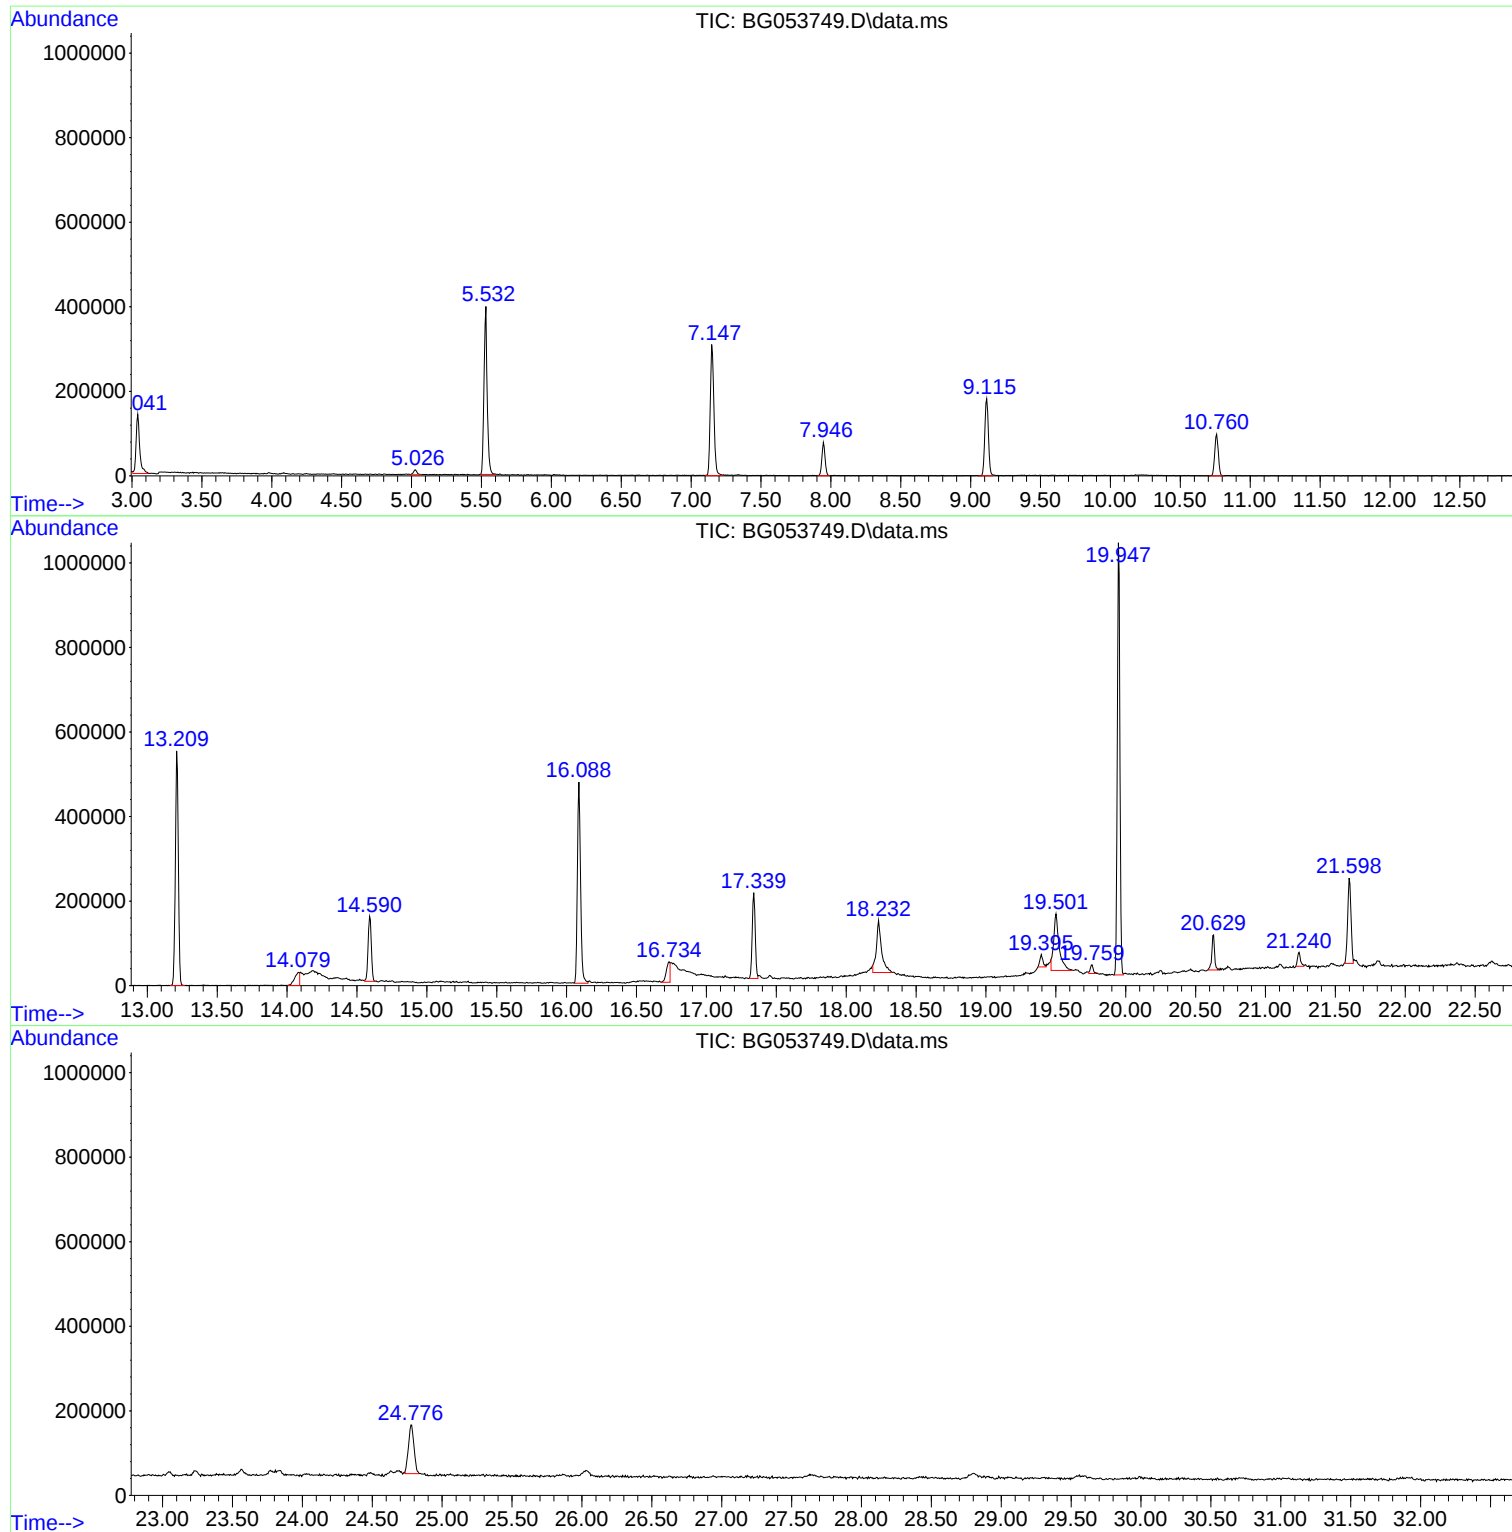

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053749.D
Acq On : 28 May 2022 13:51
Operator : CG/JU
Sample : N3080-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053749.D
Acq On : 28 May 2022 13:51
Operator : CG/JU
Sample : N3080-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc