

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
 Data File : BG053754.D
 Acq On : 28 May 2022 17:11
 Operator : CG/JU
 Sample : N3076-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RBR-671

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.038	3	8	14	rBV	214071	342207	13.99%	2.381%
2	5.523	425	431	447	rBV	562544	952775	38.96%	6.629%
3	7.144	701	707	723	rBV	591376	1054564	43.12%	7.337%
4	7.943	836	843	851	rBV	138657	236625	9.68%	1.646%
5	9.112	1034	1042	1057	rBV	370446	666190	27.24%	4.635%
6	10.757	1315	1322	1333	rBV	187242	331636	13.56%	2.307%
7	13.212	1733	1740	1751	rBV	955543	1493768	61.08%	10.393%
8	13.353	1758	1764	1770	rBV2	33609	48265	1.97%	0.336%
9	14.593	1968	1975	1981	rBV	300882	479936	19.63%	3.339%
10	16.085	2223	2229	2246	rBV	719689	1142493	46.72%	7.949%
11	17.336	2436	2442	2451	rBV	409408	569822	23.30%	3.965%
12	18.235	2591	2595	2610	rBV2	69292	170634	6.98%	1.187%
13	19.510	2809	2812	2820	rBV5	22977	47249	1.93%	0.329%
14	19.950	2881	2887	2894	rBV	1863301	2445453	100.00%	17.015%
15	21.231	3100	3105	3113	rBV	229323	351896	14.39%	2.448%
16	21.601	3162	3168	3176	rVB	393130	641866	26.25%	4.466%
17	22.012	3234	3238	3244	rBV3	29636	49556	2.03%	0.345%
18	22.371	3294	3299	3311	rVB5	91679	263861	10.79%	1.836%
19	22.652	3342	3347	3353	rVB9	16428	30244	1.24%	0.210%
20	23.387	3467	3472	3479	rVB3	54964	114191	4.67%	0.794%
21	23.598	3504	3508	3510	rBV5	21198	37887	1.55%	0.264%
22	23.833	3541	3548	3554	rBV3	326572	657035	26.87%	4.571%
23	23.898	3555	3559	3570	rVB4	58142	139512	5.70%	0.971%
24	24.333	3630	3633	3639	rBV8	14528	29710	1.21%	0.207%
25	24.556	3668	3671	3678	rBV8	14189	28321	1.16%	0.197%
26	24.773	3696	3708	3709	rBV	204966	423006	17.30%	2.943%
27	25.272	3786	3793	3798	rVB6	44021	106828	4.37%	0.743%
28	25.860	3885	3893	3903	rVB	130340	377991	15.46%	2.630%
29	25.960	3906	3910	3911	rBV2	29593	38127	1.56%	0.265%
30	26.042	3922	3924	3933	rVB7	28467	66182	2.71%	0.460%
31	26.195	3949	3950	3956	rVB5	23250	32247	1.32%	0.224%
32	26.347	3974	3976	3978	rBV2	20665	27036	1.11%	0.188%
33	27.957	4243	4250	4264	rVB3	101178	351569	14.38%	2.446%
34	28.779	4389	4390	4396	rVB4	24001	31858	1.30%	0.222%
35	28.868	4403	4405	4409	rBV4	16945	25298	1.03%	0.176%
36	29.003	4425	4428	4432	rBV5	24497	34395	1.41%	0.239%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053754.D
Acq On : 28 May 2022 17:11
Operator : CG/JU
Sample : N3076-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RBR-671

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	29.514	4513	4515	4518	rBV3	17990	27604	1.13%	0.192%
38	29.960	4584	4591	4601	rBV3	48183	187202	7.66%	1.302%
39	30.413	4666	4668	4670	rBV2	23418	29862	1.22%	0.208%
40	30.595	4695	4699	4707	rBV8	20471	66937	2.74%	0.466%
41	31.006	4768	4769	4777	rBV5	23481	51803	2.12%	0.360%
42	31.206	4800	4803	4811	rBV9	20587	44688	1.83%	0.311%
43	31.335	4821	4825	4827	rBV4	17271	33352	1.36%	0.232%
44	31.911	4921	4923	4929	rVB7	25388	32205	1.32%	0.224%
45	32.445	5012	5014	5019	rBV5	22514	30379	1.24%	0.211%
46	32.516	5024	5026	5036	rVB9	22902	28447	1.16%	0.198%


Sum of corrected areas: 14372712

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053754.D
Acq On : 28 May 2022 17:11
Operator : CG/JU
Sample : N3076-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RBR-671

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

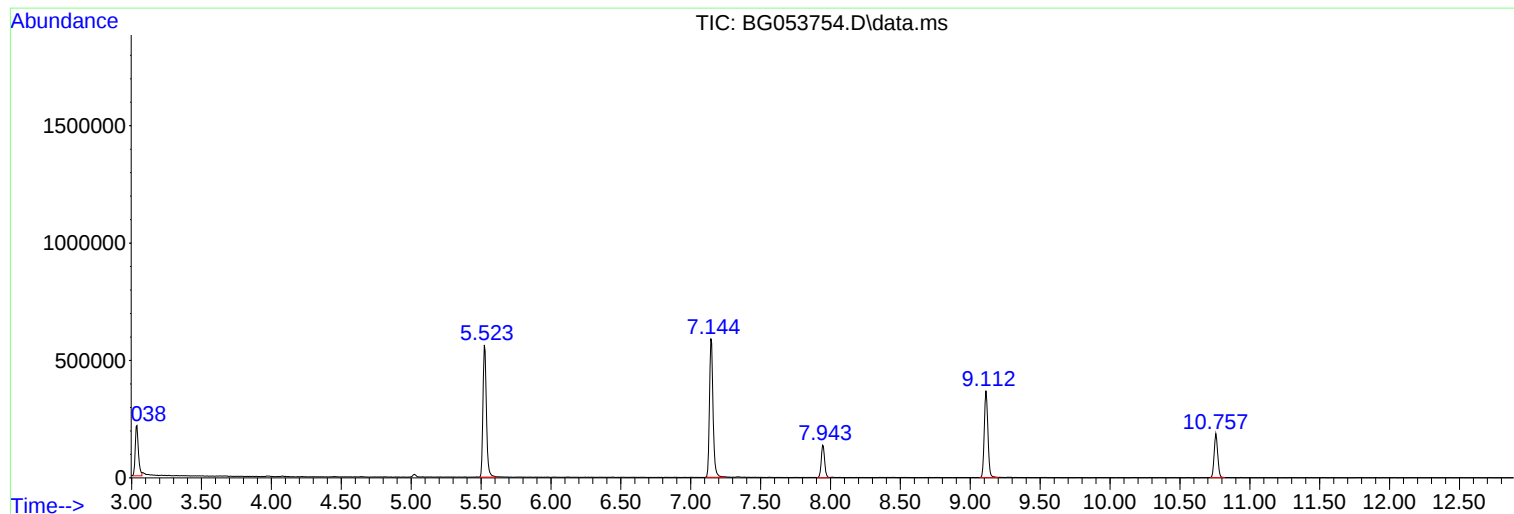

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053754.D
Acq On : 28 May 2022 17:11
Operator : CG/JU
Sample : N3076-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RBR-671

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053754.D
Acq On : 28 May 2022 17:11
Operator : CG/JU
Sample : N3076-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RBR-671

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------