

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
 Data File : BG053755.D
 Acq On : 28 May 2022 17:51
 Operator : CG/JU
 Sample : N3041-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 2147

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053755.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.042	3	9	22	rBV	196655	358254	19.61%	2.333%
2	3.618	103	107	111	rBV	13917	18940	1.04%	0.123%
3	4.628	273	279	284	rBV3	15122	26455	1.45%	0.172%
4	5.527	425	432	447	rBV	544408	900879	49.31%	5.866%
5	7.089	691	698	702	rBV6	10055	22975	1.26%	0.150%
6	7.148	702	708	718	rVV	560736	979122	53.60%	6.375%
7	7.947	834	844	851	rBV	154275	274767	15.04%	1.789%
8	9.116	1035	1043	1050	rBV	343901	632973	34.65%	4.121%
9	10.755	1310	1322	1329	rBV	218126	419596	22.97%	2.732%
10	10.808	1329	1331	1339	rVB2	14030	21899	1.20%	0.143%
11	10.914	1344	1349	1353	rVB2	15021	22339	1.22%	0.145%
12	11.777	1491	1496	1501	rBV2	26326	41189	2.25%	0.268%
13	12.171	1557	1563	1570	rBV	22024	37319	2.04%	0.243%
14	12.418	1597	1605	1613	rVB3	17332	38278	2.10%	0.249%
15	12.641	1635	1643	1648	rVV	13997	25727	1.41%	0.168%
16	13.122	1719	1725	1730	rVB	18449	30247	1.66%	0.197%
17	13.211	1730	1740	1748	rBV	1037589	1617352	88.53%	10.531%
18	13.404	1768	1773	1781	rBV2	33340	59117	3.24%	0.385%
19	13.910	1855	1859	1863	rBV	20791	36127	1.98%	0.235%
20	13.963	1863	1868	1874	rVB3	16674	29404	1.61%	0.191%
21	14.062	1881	1885	1890	rBV	23362	32816	1.80%	0.214%
22	14.479	1951	1956	1961	rBV	36018	47739	2.61%	0.311%
23	14.591	1964	1975	1982	rBV	381358	623768	34.14%	4.061%
24	14.673	1986	1989	1993	rVB6	14545	21371	1.17%	0.139%
25	14.808	2006	2012	2018	rVB8	11925	25612	1.40%	0.167%
26	14.991	2038	2043	2048	rVB4	26517	46373	2.54%	0.302%
27	15.067	2052	2056	2059	rBV2	14048	19227	1.05%	0.125%
28	15.208	2074	2080	2085	rBV3	21394	36033	1.97%	0.235%
29	15.261	2085	2089	2093	rVB2	12878	20309	1.11%	0.132%
30	15.378	2102	2109	2113	rBV4	18580	33167	1.82%	0.216%
31	15.425	2113	2117	2121	rVB	31465	43687	2.39%	0.284%
32	15.637	2148	2153	2155	rBV5	12216	19424	1.06%	0.126%
33	15.836	2183	2187	2195	rVV8	15481	34446	1.89%	0.224%
34	15.930	2197	2203	2210	rBV5	15091	33689	1.84%	0.219%
35	16.083	2224	2229	2242	rBV	565144	961188	52.61%	6.258%
36	16.289	2260	2264	2266	rBV	40708	54198	2.97%	0.353%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
 Data File : BG053755.D
 Acq On : 28 May 2022 17:51
 Operator : CG/JU
 Sample : N3041-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 2147

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.312	2266	2268	2274	rVB2	38735	47209	2.58%	0.307%
38	16.694	2329	2333	2340	rVB7	15164	22740	1.24%	0.148%
39	16.870	2356	2363	2366	rBV9	17430	32510	1.78%	0.212%
40	16.994	2380	2384	2390	rBV3	29298	57387	3.14%	0.374%
41	17.082	2393	2399	2403	rVV2	48131	64598	3.54%	0.421%
42	17.164	2410	2413	2421	rVB6	18250	29776	1.63%	0.194%
43	17.340	2436	2443	2447	rBV	410917	638857	34.97%	4.160%
44	17.381	2447	2450	2457	rVV	115317	167127	9.15%	1.088%
45	17.475	2461	2466	2469	rVB	13556	24144	1.32%	0.157%
46	17.528	2469	2475	2480	rBV4	17508	43885	2.40%	0.286%
47	17.628	2486	2492	2493	rBV5	16214	25933	1.42%	0.169%
48	17.746	2508	2512	2519	rBV3	18590	45073	2.47%	0.293%
49	17.822	2521	2525	2528	rVB2	38654	48033	2.63%	0.313%
50	17.992	2550	2554	2558	rBV	46098	54558	2.99%	0.355%
51	18.239	2587	2596	2597	rBV2	61676	143208	7.84%	0.932%
52	18.263	2597	2600	2606	rVB3	107492	172934	9.47%	1.126%
53	18.398	2619	2623	2628	rBV3	68405	102273	5.60%	0.666%
54	18.445	2628	2631	2635	rVB	37812	56947	3.12%	0.371%
55	18.509	2638	2642	2648	rBV3	42971	71944	3.94%	0.468%
56	18.568	2648	2652	2655	rVV6	16311	24886	1.36%	0.162%
57	18.609	2655	2659	2663	rVB5	25860	39998	2.19%	0.260%
58	18.709	2672	2676	2682	rBV2	52446	93571	5.12%	0.609%
59	18.762	2682	2685	2693	rVB6	28090	57955	3.17%	0.377%
60	18.956	2715	2718	2723	rVB2	32195	42735	2.34%	0.278%
61	19.009	2724	2727	2731	rBV	35561	44784	2.45%	0.292%
62	19.050	2731	2734	2738	rVB	27663	35452	1.94%	0.231%
63	19.132	2742	2748	2752	rBV2	112937	199577	10.92%	1.299%
64	19.220	2760	2763	2767	rVB	31340	38352	2.10%	0.250%
65	19.267	2767	2771	2777	rBV3	29859	61146	3.35%	0.398%
66	19.390	2787	2792	2798	rVB2	200659	289657	15.86%	1.886%
67	19.449	2798	2802	2805	rBV	42012	50953	2.79%	0.332%
68	19.508	2805	2812	2814	rBV6	38938	70967	3.88%	0.462%
69	19.719	2844	2848	2850	rBV3	47507	60891	3.33%	0.396%
70	19.755	2850	2854	2862	rVV	150530	259469	14.20%	1.689%
71	19.825	2862	2866	2872	rVB	47695	75194	4.12%	0.490%
72	19.949	2882	2887	2892	rVB	1472864	1826838	100.00%	11.895%
73	20.060	2903	2906	2909	rBV2	49506	74916	4.10%	0.488%
74	20.095	2910	2912	2918	rVB3	47920	65352	3.58%	0.426%
75	20.242	2934	2937	2943	rVB	72783	104018	5.69%	0.677%
76	20.495	2976	2980	2985	rVB4	41419	65265	3.57%	0.425%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
 Data File : BG053755.D
 Acq On : 28 May 2022 17:51
 Operator : CG/JU
 Sample : N3041-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 2147

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	21.006	3064	3067	3073	rVB	49888	71957	3.94%	0.469%
78	21.182	3087	3097	3101	rBV3	65189	186898	10.23%	1.217%
79	21.235	3102	3106	3110	rVV3	88039	122187	6.69%	0.796%
80	21.476	3145	3147	3152	rVB3	42357	39534	2.16%	0.257%
81	21.599	3161	3168	3173	rBV2	397387	751463	41.13%	4.893%
82	21.640	3173	3175	3189	rVB2	73490	179854	9.85%	1.171%
83	22.833	3376	3378	3382	rBV5	20364	33468	1.83%	0.218%
84	23.773	3532	3538	3539	rBV2	49395	88271	4.83%	0.575%
85	24.037	3580	3583	3584	rBV2	22917	24405	1.34%	0.159%
86	24.777	3701	3709	3721	rBV2	192546	550600	30.14%	3.585%
87	26.034	3920	3923	3926	rBV5	17247	27228	1.49%	0.177%
88	26.275	3962	3964	3967	rBV4	20268	28985	1.59%	0.189%
89	29.882	4574	4578	4580	rBV5	12885	20227	1.11%	0.132%
90	29.947	4585	4589	4591	rBV5	22078	41670	2.28%	0.271%
91	30.387	4662	4664	4673	rVB10	16309	28091	1.54%	0.183%
92	30.940	4755	4758	4761	rBV4	19119	33606	1.84%	0.219%
93	31.098	4782	4785	4789	rBV5	19942	29163	1.60%	0.190%
94	31.151	4792	4794	4800	rVB6	18136	23420	1.28%	0.152%




Sum of corrected areas: 15358145

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053755.D
Acq On : 28 May 2022 17:51
Operator : CG/JU
Sample : N3041-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
2147

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

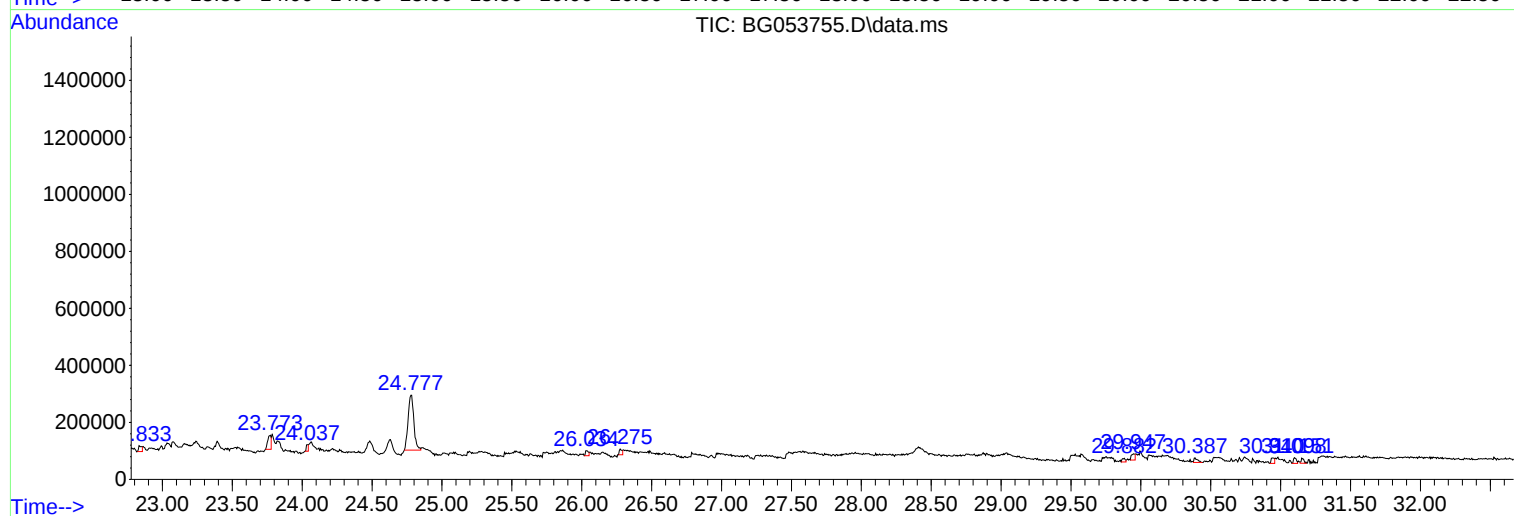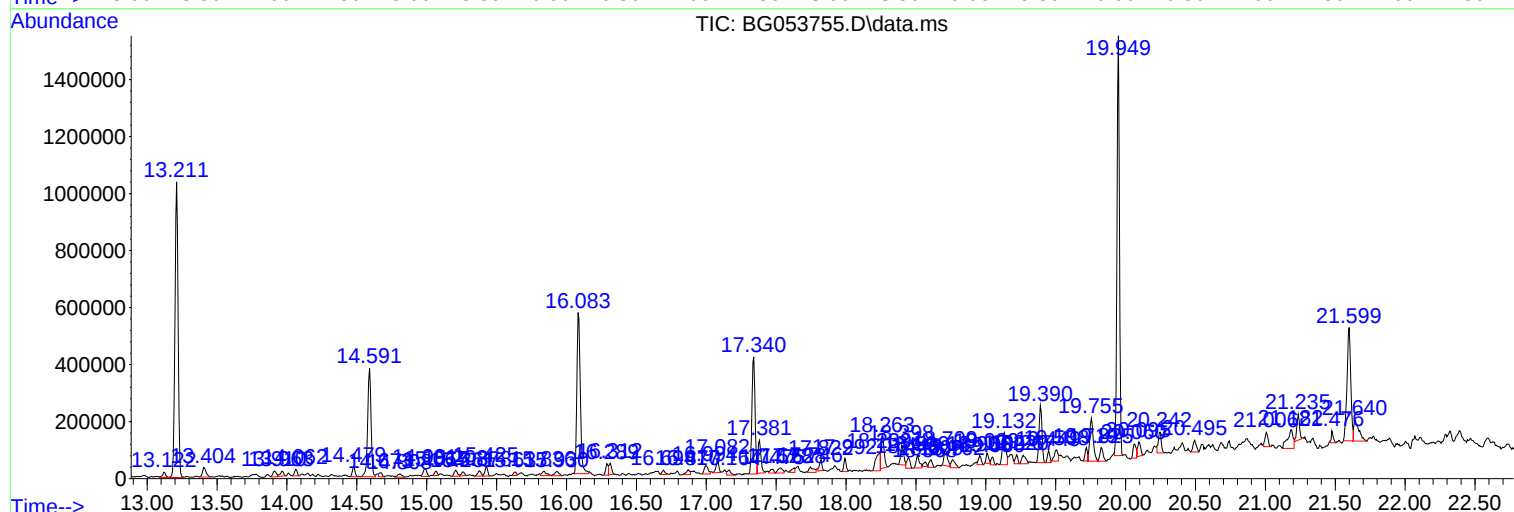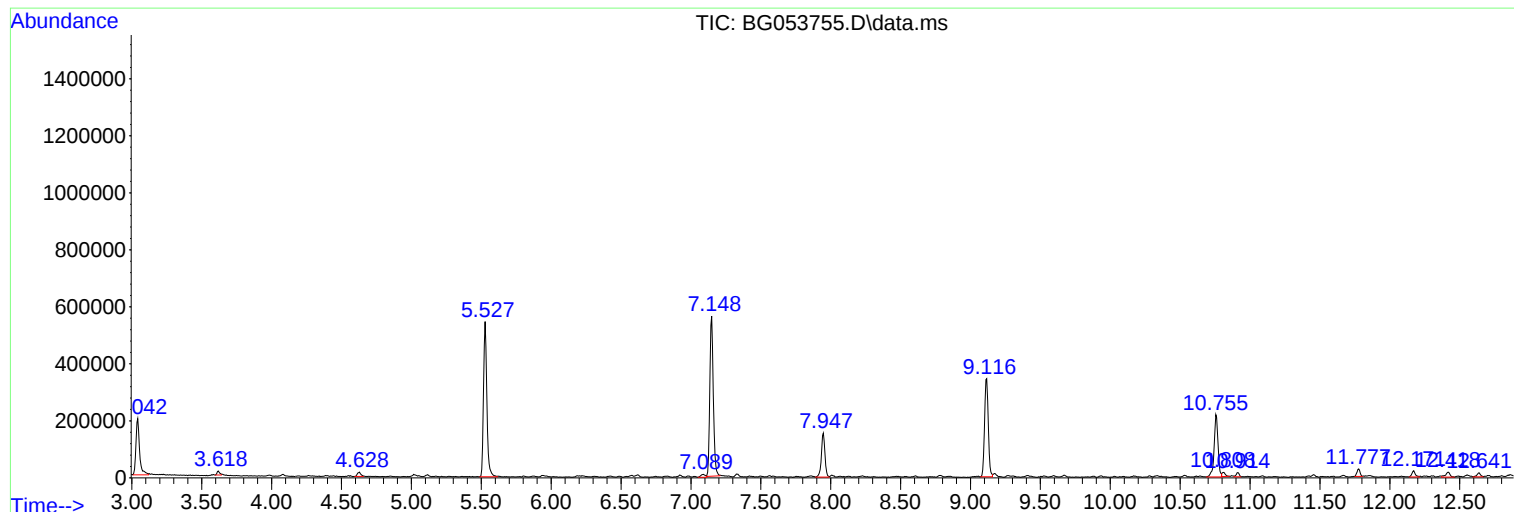

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053755.D
Acq On : 28 May 2022 17:51
Operator : CG/JU
Sample : N3041-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
2147

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053755.D
Acq On : 28 May 2022 17:51
Operator : CG/JU
Sample : N3041-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
2147

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------