

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052822\  
 Data File : BG053756.D  
 Acq On : 28 May 2022 18:31  
 Operator : CG/JU  
 Sample : N3080-01  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 WC-4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053756.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.035       | 3             | 8           | 28           | rBV      | 194863         | 386079        | 17.77%          | 1.962%        |
| 2         | 5.020       | 339           | 346         | 356          | rBV4     | 15256          | 35142         | 1.62%           | 0.179%        |
| 3         | 5.526       | 425           | 432         | 446          | rBV      | 651335         | 1096816       | 50.49%          | 5.574%        |
| 4         | 7.147       | 701           | 708         | 725          | rBV      | 684207         | 1201942       | 55.33%          | 6.108%        |
| 5         | 7.946       | 837           | 844         | 852          | rBV      | 167625         | 283298        | 13.04%          | 1.440%        |
| 6         | 9.115       | 1035          | 1043        | 1057         | rBV      | 428799         | 791774        | 36.45%          | 4.024%        |
| 7         | 10.754      | 1313          | 1322        | 1330         | rBV      | 203683         | 387598        | 17.84%          | 1.970%        |
| 8         | 13.209      | 1733          | 1740        | 1749         | rBV      | 1093355        | 1713778       | 78.89%          | 8.709%        |
| 9         | 14.590      | 1965          | 1975        | 1981         | rBV      | 360995         | 569812        | 26.23%          | 2.896%        |
| 10        | 14.654      | 1981          | 1986        | 1995         | rVB2     | 21240          | 36654         | 1.69%           | 0.186%        |
| 11        | 14.989      | 2036          | 2043        | 2049         | rBV2     | 20196          | 33376         | 1.54%           | 0.170%        |
| 12        | 15.641      | 2146          | 2154        | 2158         | rBV3     | 29305          | 49042         | 2.26%           | 0.249%        |
| 13        | 15.935      | 2198          | 2204        | 2211         | rVB2     | 15366          | 26824         | 1.23%           | 0.136%        |
| 14        | 16.088      | 2224          | 2230        | 2244         | rBV      | 755358         | 1223585       | 56.32%          | 6.218%        |
| 15        | 16.869      | 2355          | 2363        | 2367         | rBV5     | 13538          | 28531         | 1.31%           | 0.145%        |
| 16        | 16.998      | 2380          | 2385        | 2392         | rVB4     | 15050          | 25078         | 1.15%           | 0.127%        |
| 17        | 17.081      | 2392          | 2399        | 2403         | rVV5     | 14916          | 35143         | 1.62%           | 0.179%        |
| 18        | 17.157      | 2405          | 2412        | 2421         | rVB2     | 24820          | 51500         | 2.37%           | 0.262%        |
| 19        | 17.339      | 2436          | 2443        | 2446         | rBV      | 441436         | 648303        | 29.84%          | 3.295%        |
| 20        | 17.380      | 2446          | 2450        | 2456         | rVV      | 446208         | 631436        | 29.07%          | 3.209%        |
| 21        | 17.468      | 2459          | 2465        | 2471         | rVV      | 109992         | 183539        | 8.45%           | 0.933%        |
| 22        | 17.744      | 2504          | 2512        | 2522         | rBV4     | 22043          | 70006         | 3.22%           | 0.356%        |
| 23        | 17.921      | 2538          | 2542        | 2549         | rVB7     | 13095          | 28883         | 1.33%           | 0.147%        |
| 24        | 18.214      | 2587          | 2592        | 2594         | rBV      | 63919          | 98372         | 4.53%           | 0.500%        |
| 25        | 18.261      | 2597          | 2600        | 2607         | rVB      | 103775         | 156068        | 7.18%           | 0.793%        |
| 26        | 18.344      | 2609          | 2614        | 2620         | rVB      | 40015          | 59395         | 2.73%           | 0.302%        |
| 27        | 18.408      | 2620          | 2625        | 2629         | rBV3     | 88692          | 170772        | 7.86%           | 0.868%        |
| 28        | 18.708      | 2670          | 2676        | 2681         | rBV      | 55525          | 83192         | 3.83%           | 0.423%        |
| 29        | 18.761      | 2681          | 2685        | 2689         | rVB3     | 24084          | 34104         | 1.57%           | 0.173%        |
| 30        | 18.960      | 2715          | 2719        | 2722         | rBV3     | 18727          | 22660         | 1.04%           | 0.115%        |
| 31        | 19.131      | 2743          | 2748        | 2753         | rBV2     | 47066          | 95191         | 4.38%           | 0.484%        |
| 32        | 19.272      | 2767          | 2772        | 2779         | rBV4     | 32346          | 69648         | 3.21%           | 0.354%        |
| 33        | 19.395      | 2786          | 2793        | 2799         | rBV      | 764752         | 1150550       | 52.96%          | 5.847%        |
| 34        | 19.501      | 2806          | 2811        | 2817         | rBV8     | 21557          | 55983         | 2.58%           | 0.285%        |
| 35        | 19.636      | 2830          | 2834        | 2844         | rVB      | 37134          | 75076         | 3.46%           | 0.382%        |
| 36        | 19.724      | 2844          | 2849        | 2850         | rBV      | 144616         | 188639        | 8.68%           | 0.959%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052822\  
 Data File : BG053756.D  
 Acq On : 28 May 2022 18:31  
 Operator : CG/JU  
 Sample : N3080-01  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 WC-4

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG050522.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|    |        |      |      |      |      |         |         |         |         |
|----|--------|------|------|------|------|---------|---------|---------|---------|
| 37 | 19.753 | 2850 | 2854 | 2862 | rVV  | 650558  | 958804  | 44.14%  | 4.873%  |
| 38 | 19.824 | 2862 | 2866 | 2873 | rVB3 | 42937   | 69604   | 3.20%   | 0.354%  |
| 39 | 19.947 | 2880 | 2887 | 2892 | rBV  | 1674275 | 2172403 | 100.00% | 11.040% |
| 40 | 20.000 | 2892 | 2896 | 2903 | rVB2 | 34600   | 55720   | 2.56%   | 0.283%  |
| 41 | 20.071 | 2904 | 2908 | 2916 | rBV2 | 45572   | 119949  | 5.52%   | 0.610%  |
| 42 | 20.247 | 2928 | 2938 | 2943 | rVB2 | 97545   | 225284  | 10.37%  | 1.145%  |
| 43 | 20.341 | 2951 | 2954 | 2958 | rBV  | 47533   | 65794   | 3.03%   | 0.334%  |
| 44 | 20.405 | 2959 | 2965 | 2969 | rBV2 | 62334   | 122871  | 5.66%   | 0.624%  |
| 45 | 20.546 | 2985 | 2989 | 2993 | rBV  | 37060   | 57104   | 2.63%   | 0.290%  |
| 46 | 20.588 | 2993 | 2996 | 2999 | rVV3 | 41875   | 66757   | 3.07%   | 0.339%  |
| 47 | 20.623 | 3000 | 3002 | 3008 | rVB2 | 56448   | 72019   | 3.32%   | 0.366%  |
| 48 | 21.005 | 3064 | 3067 | 3071 | rVB  | 51167   | 66312   | 3.05%   | 0.337%  |
| 49 | 21.187 | 3096 | 3098 | 3101 | rBV2 | 29282   | 26545   | 1.22%   | 0.135%  |
| 50 | 21.228 | 3101 | 3105 | 3109 | rVB3 | 85950   | 115636  | 5.32%   | 0.588%  |
| 51 | 21.598 | 3160 | 3168 | 3173 | rBV3 | 464826  | 1167055 | 53.72%  | 5.931%  |
| 52 | 21.645 | 3173 | 3176 | 3182 | rVB  | 235667  | 329032  | 15.15%  | 1.672%  |
| 53 | 22.003 | 3233 | 3237 | 3238 | rBV3 | 55223   | 71970   | 3.31%   | 0.366%  |
| 54 | 23.772 | 3531 | 3538 | 3546 | rBV2 | 191099  | 632683  | 29.12%  | 3.215%  |
| 55 | 24.488 | 3655 | 3660 | 3673 | rVB  | 114128  | 310121  | 14.28%  | 1.576%  |
| 56 | 24.629 | 3677 | 3684 | 3696 | rVB  | 179613  | 525291  | 24.18%  | 2.670%  |
| 57 | 24.776 | 3702 | 3709 | 3718 | rBV2 | 213607  | 572326  | 26.35%  | 2.909%  |
| 58 | 27.878 | 4234 | 4237 | 4238 | rBV3 | 25859   | 34735   | 1.60%   | 0.177%  |
| 59 | 28.236 | 4295 | 4298 | 4299 | rBV3 | 33479   | 41541   | 1.91%   | 0.211%  |




Sum of corrected areas: 19677345

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052822\  
Data File : BG053756.D  
Acq On : 28 May 2022 18:31  
Operator : CG/JU  
Sample : N3080-01  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
WC-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG050522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

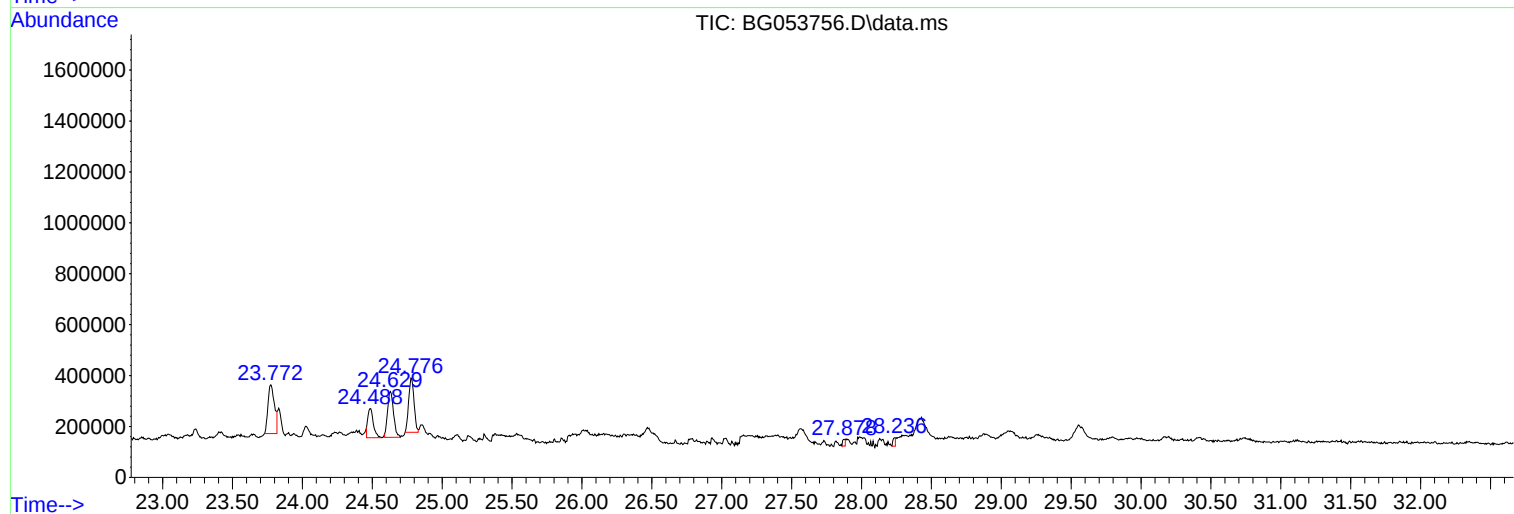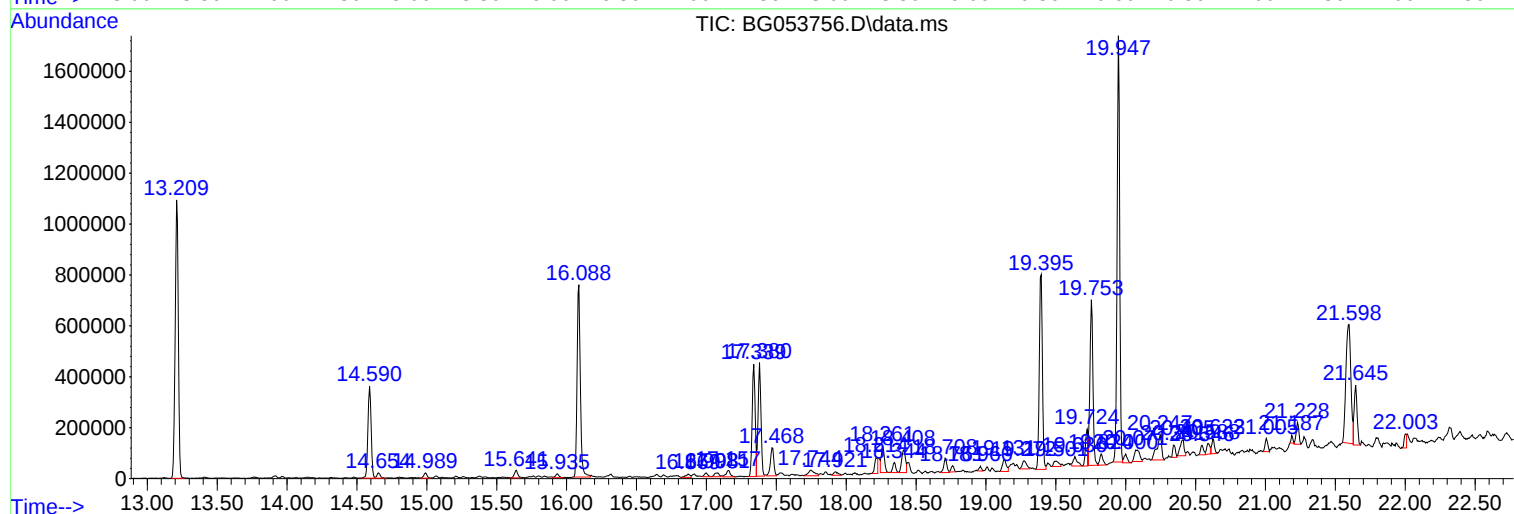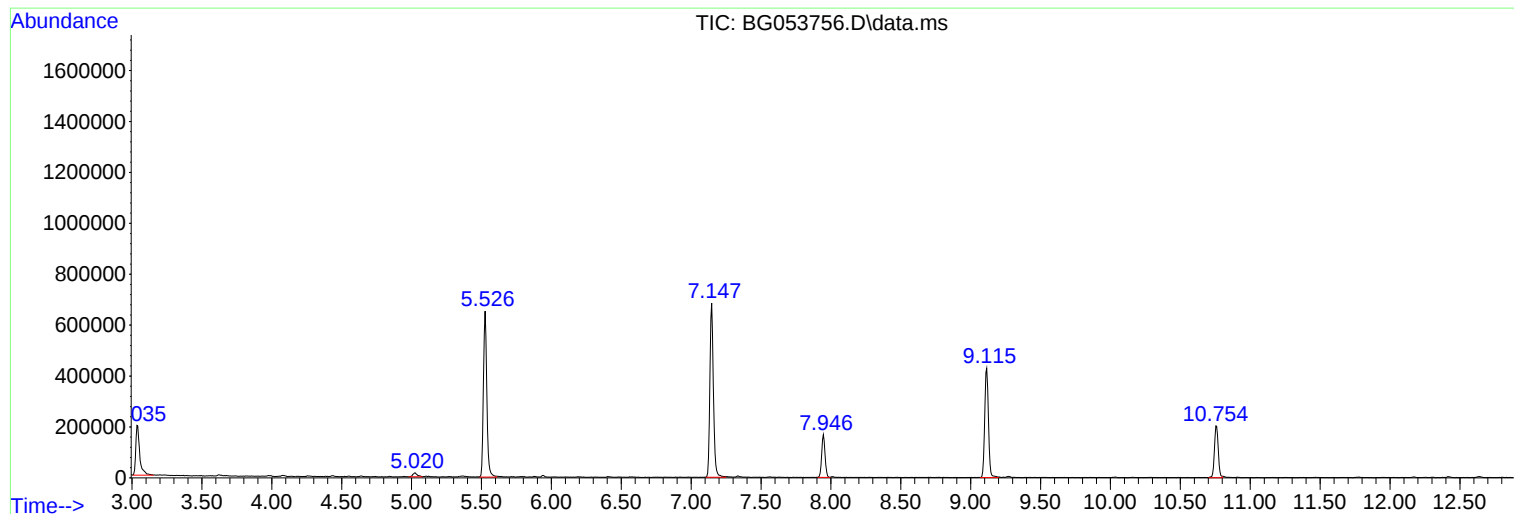

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052822\  
Data File : BG053756.D  
Acq On : 28 May 2022 18:31  
Operator : CG/JU  
Sample : N3080-01  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
WC-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG050522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG052822\  
Data File : BG053756.D  
Acq On : 28 May 2022 18:31  
Operator : CG/JU  
Sample : N3080-01  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
WC-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG050522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       | #        | RT Resp Conc          |