

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
 Data File : BG053757.D
 Acq On : 28 May 2022 19:11
 Operator : CG/JU
 Sample : N3042-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 303

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053757.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.038	3	8	26	rVB	262817	490812	19.70%	3.208%
2	5.024	341	346	353	rBV2	21373	34065	1.37%	0.223%
3	5.529	425	432	444	rBV	584699	980377	39.35%	6.407%
4	7.144	701	707	725	rBV	591413	1069757	42.94%	6.991%
5	7.949	838	844	851	rVB	184998	311221	12.49%	2.034%
6	9.112	1035	1042	1050	rBV	382367	693325	27.83%	4.531%
7	10.757	1311	1322	1332	rVB	252235	461181	18.51%	3.014%
8	12.384	1592	1599	1611	rBV6	17723	49174	1.97%	0.321%
9	12.807	1666	1671	1675	rBV3	36149	58678	2.36%	0.383%
10	13.119	1721	1724	1730	rVB	37393	52006	2.09%	0.340%
11	13.213	1730	1740	1748	rBV	643266	1045254	41.96%	6.831%
12	13.401	1769	1772	1780	rVB4	30245	54385	2.18%	0.355%
13	13.859	1846	1850	1857	rBV9	39188	90749	3.64%	0.593%
14	14.065	1881	1885	1889	rBV2	143256	210300	8.44%	1.374%
15	14.329	1927	1930	1931	rBV2	32879	38464	1.54%	0.251%
16	14.487	1952	1957	1964	rBV4	100656	257285	10.33%	1.681%
17	14.552	1966	1968	1969	rVV	88713	79623	3.20%	0.520%
18	14.593	1971	1975	1982	rVB	410376	679039	27.26%	4.438%
19	15.104	2059	2062	2067	rVB2	138762	198884	7.98%	1.300%
20	15.844	2184	2188	2198	rVB	442838	745539	29.93%	4.872%
21	16.091	2227	2230	2235	rVB	480056	606630	24.35%	3.965%
22	16.326	2266	2270	2274	rVB	1055884	1444073	57.97%	9.438%
23	17.149	2406	2410	2421	rVB	1597332	2491269	100.00%	16.282%
24	17.348	2440	2444	2449	rVB2	489783	797636	32.02%	5.213%
25	19.957	2885	2888	2895	rVB	801767	1094905	43.95%	7.156%
26	21.607	3165	3169	3174	rVB	401913	605817	24.32%	3.959%
27	24.785	3703	3710	3719	rVB	234111	660562	26.52%	4.317%




Sum of corrected areas: 15301010

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053757.D
Acq On : 28 May 2022 19:11
Operator : CG/JU
Sample : N3042-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
303

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

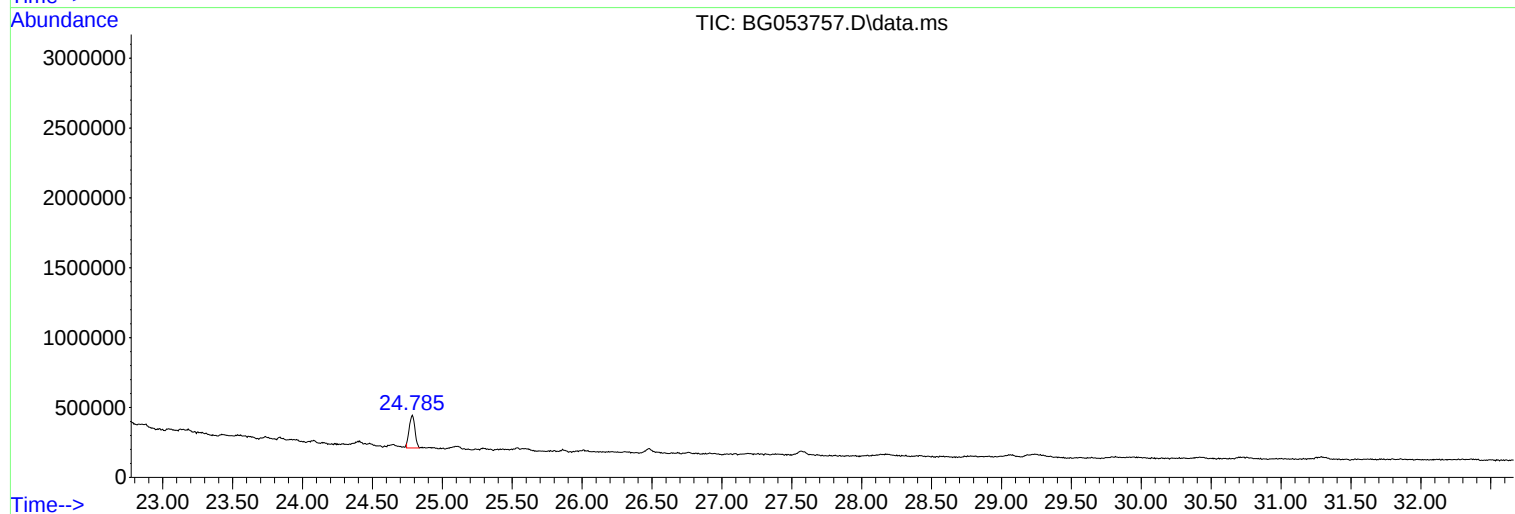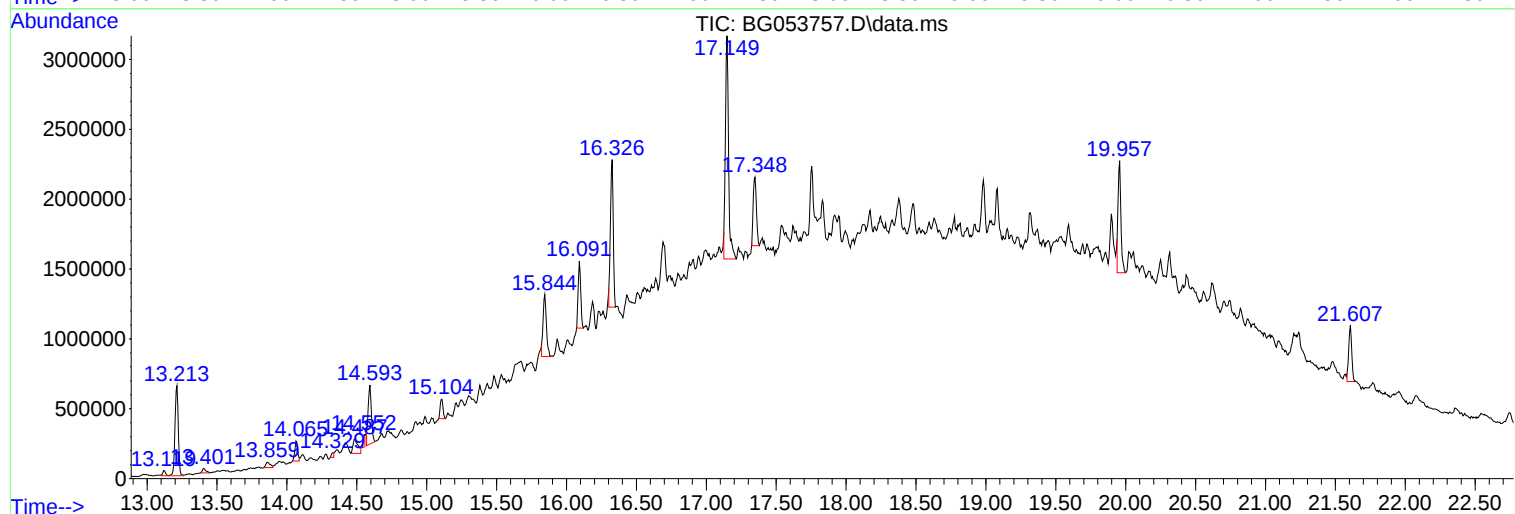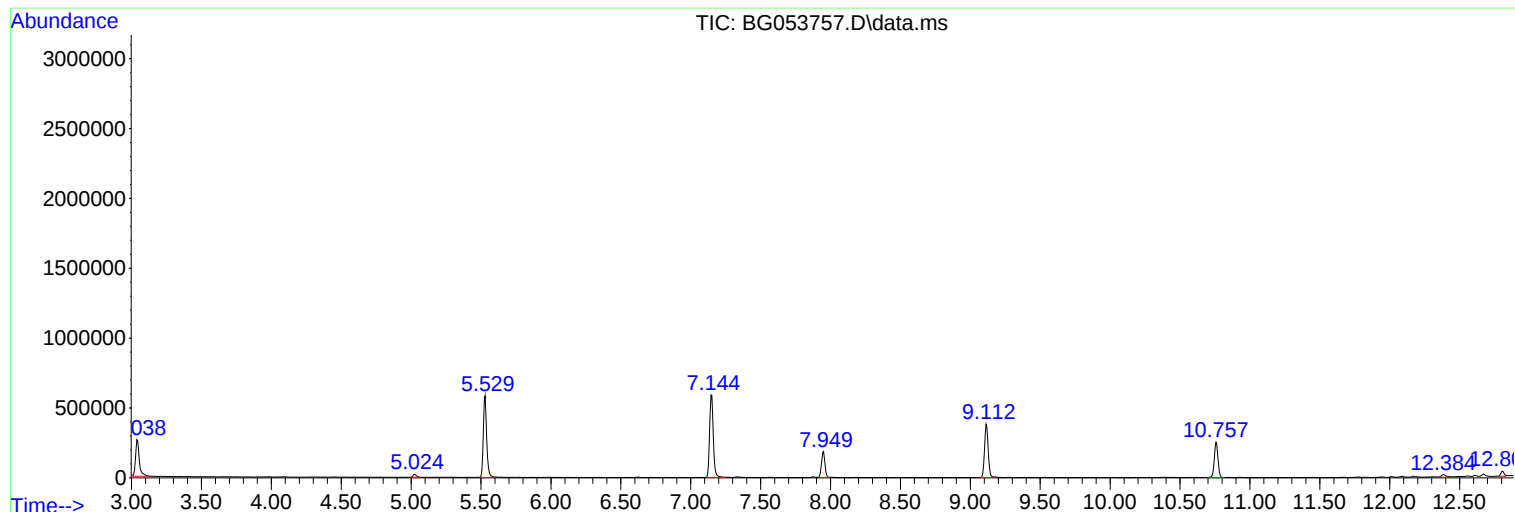

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053757.D
Acq On : 28 May 2022 19:11
Operator : CG/JU
Sample : N3042-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
303

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053757.D
Acq On : 28 May 2022 19:11
Operator : CG/JU
Sample : N3042-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
303

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------