

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
 Data File : BG053762.D
 Acq On : 28 May 2022 22:31
 Operator : CG/JU
 Sample : N3055-03 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ETGI-329

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.947	838	844	852	rBV	215940	376741	3.60%	0.889%
2	10.761	1310	1323	1329	rBV	296517	660557	6.31%	1.559%
3	11.454	1432	1441	1447	rBV8	85300	197547	1.89%	0.466%
4	11.671	1472	1478	1485	rBV9	70845	165882	1.58%	0.392%
5	11.947	1517	1525	1531	rBV7	128754	308670	2.95%	0.729%
6	12.494	1614	1618	1623	rBV5	145340	278314	2.66%	0.657%
7	12.676	1644	1649	1658	rBV4	307947	592790	5.66%	1.399%
8	12.746	1658	1661	1665	rBV3	162173	269942	2.58%	0.637%
9	13.034	1707	1710	1715	rBV	253282	364224	3.48%	0.860%
10	13.134	1724	1727	1732	rVB2	425670	579802	5.53%	1.369%
11	13.204	1733	1739	1747	rVV8	330189	961514	9.18%	2.270%
12	13.381	1766	1769	1772	rBV3	416776	615685	5.88%	1.453%
13	14.027	1875	1879	1883	rBV	1608158	2455887	23.44%	5.798%
14	14.350	1930	1934	1937	rBV3	927319	1701705	16.24%	4.017%
15	14.444	1945	1950	1956	rVB3	2614514	4819866	46.01%	11.378%
16	14.579	1969	1973	1977	rBV4	1617610	3281855	31.33%	7.747%
17	14.632	1979	1982	1987	rVB	2933383	4232299	40.40%	9.991%
18	16.377	2275	2279	2290	rVB	6282835	10476215	100.00%	24.731%
19	17.205	2416	2420	2429	rVB	5731016	10020987	95.65%	23.656%




Sum of corrected areas: 42360482

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053762.D
Acq On : 28 May 2022 22:31
Operator : CG/JU
Sample : N3055-03 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ETGI-329

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

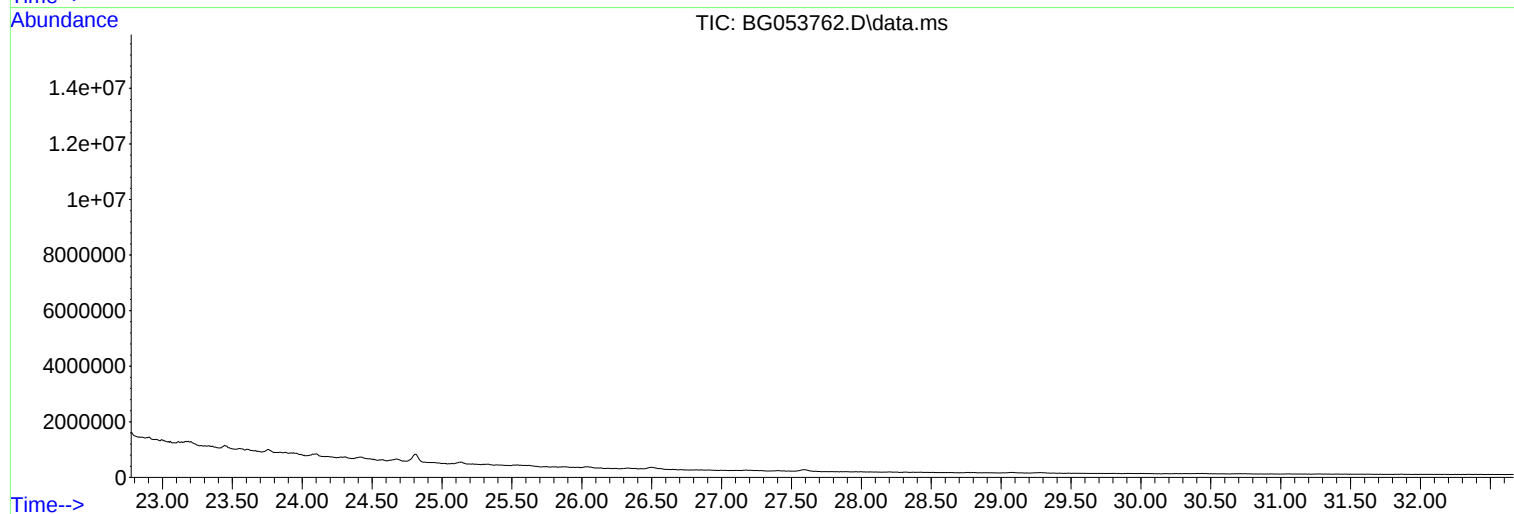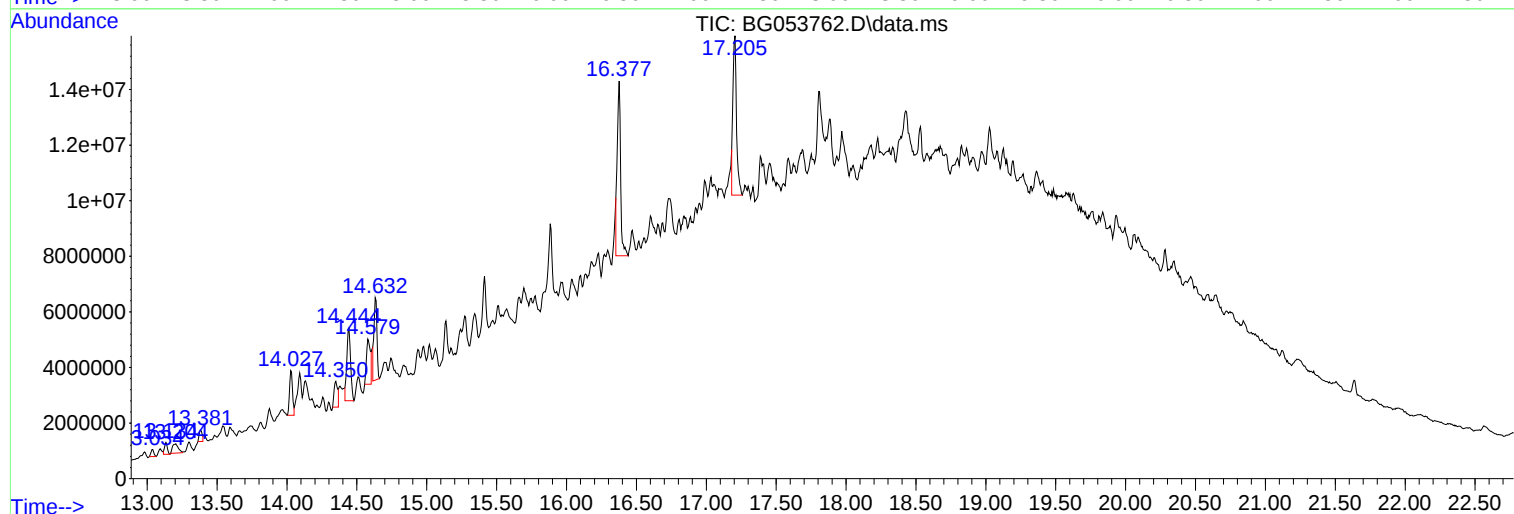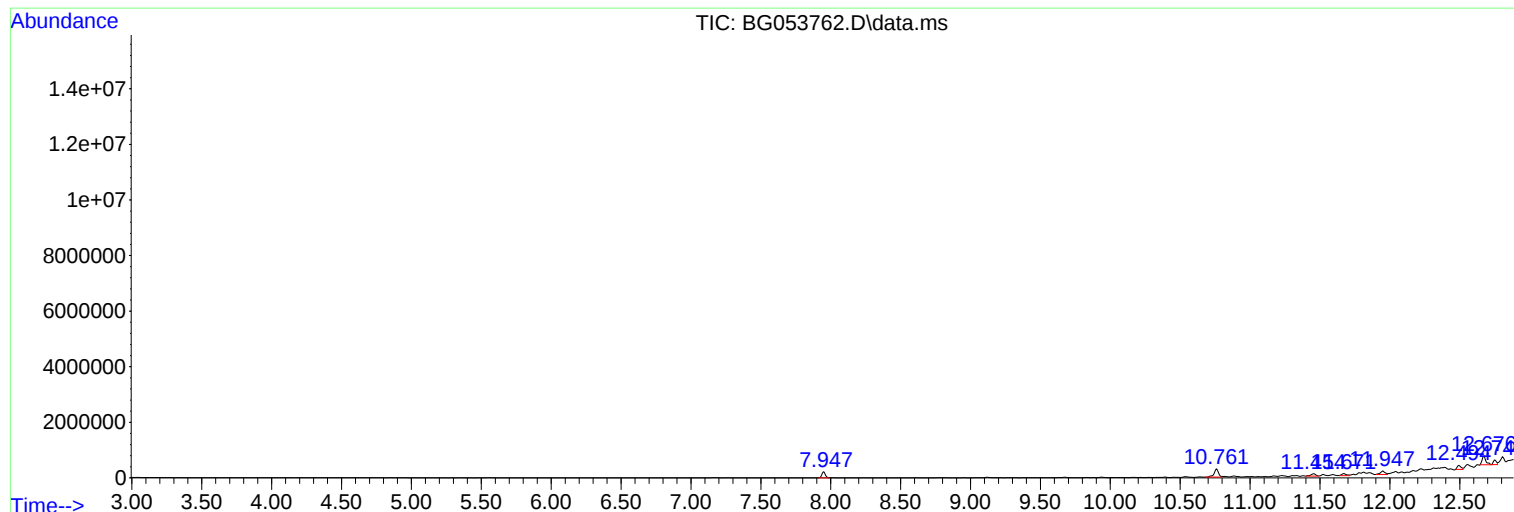

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053762.D
Acq On : 28 May 2022 22:31
Operator : CG/JU
Sample : N3055-03 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ETGI-329

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053762.D
Acq On : 28 May 2022 22:31
Operator : CG/JU
Sample : N3055-03 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ETGI-329

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc