
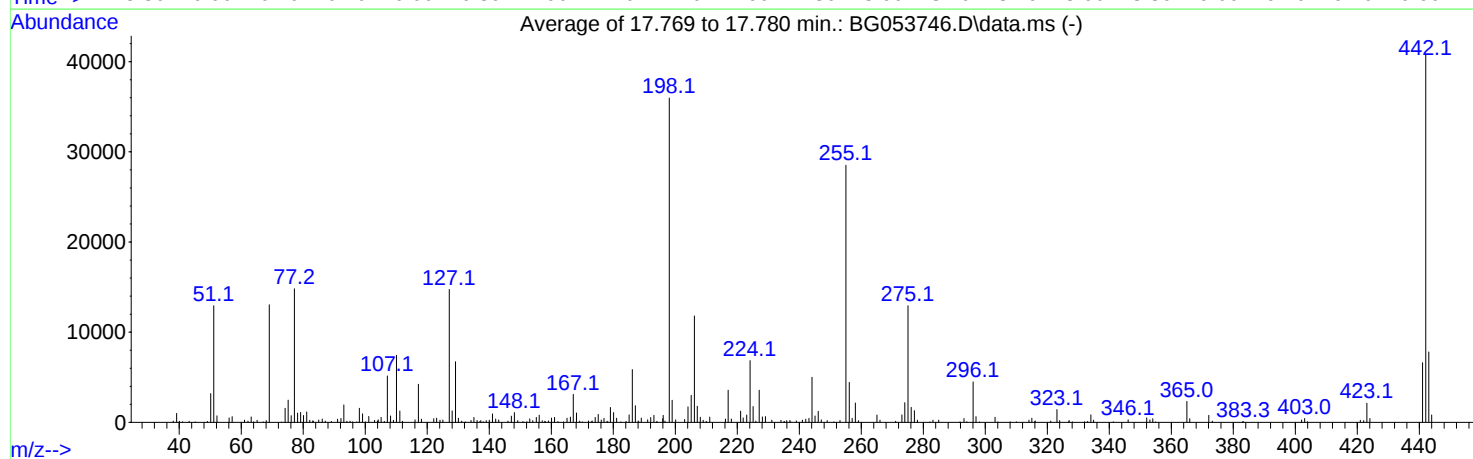


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
 Data File : BG053746.D
 Acq On : 28 May 2022 10:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun May 29 02:17:06 2022

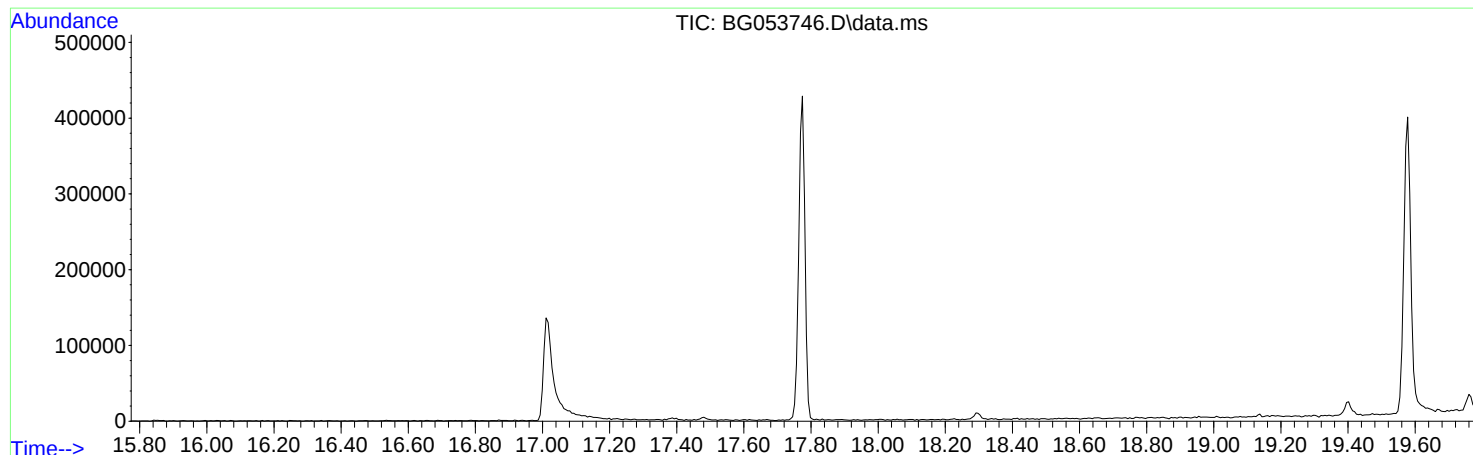




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	12936	PASS
68	69	0.00	2	1.5	194	PASS
69	198	0.00	100	36.3	13043	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	14738	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35973	PASS
199	198	5	9	6.8	2455	PASS
275	198	10	60	35.9	12930	PASS
365	198	1	100	6.4	2318	PASS
441	198	0.01	100	18.4	6624	PASS
442	442	50	100	100.0	40797	PASS
443	442	15	24	19.1	7803	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053746.D
Acq On : 28 May 2022 10:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 28 11:04:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

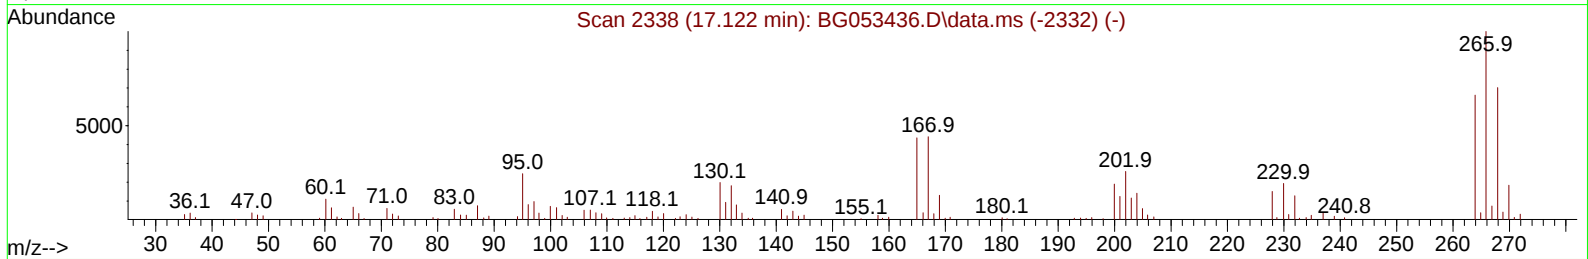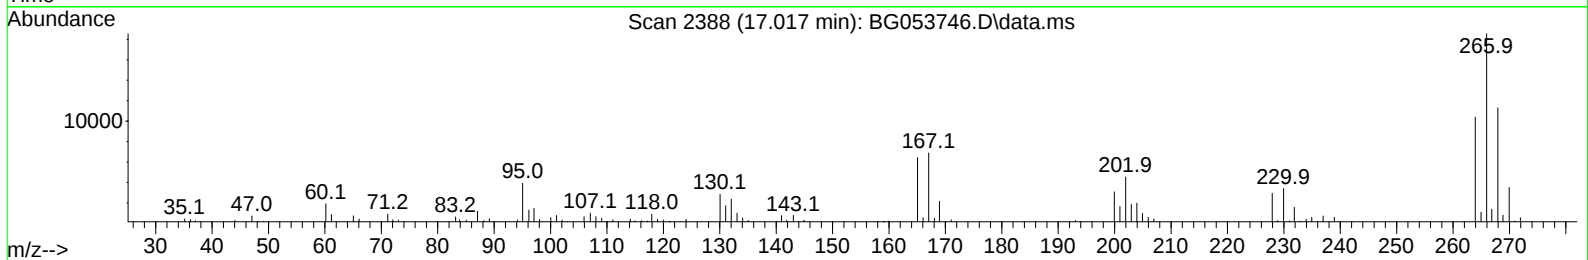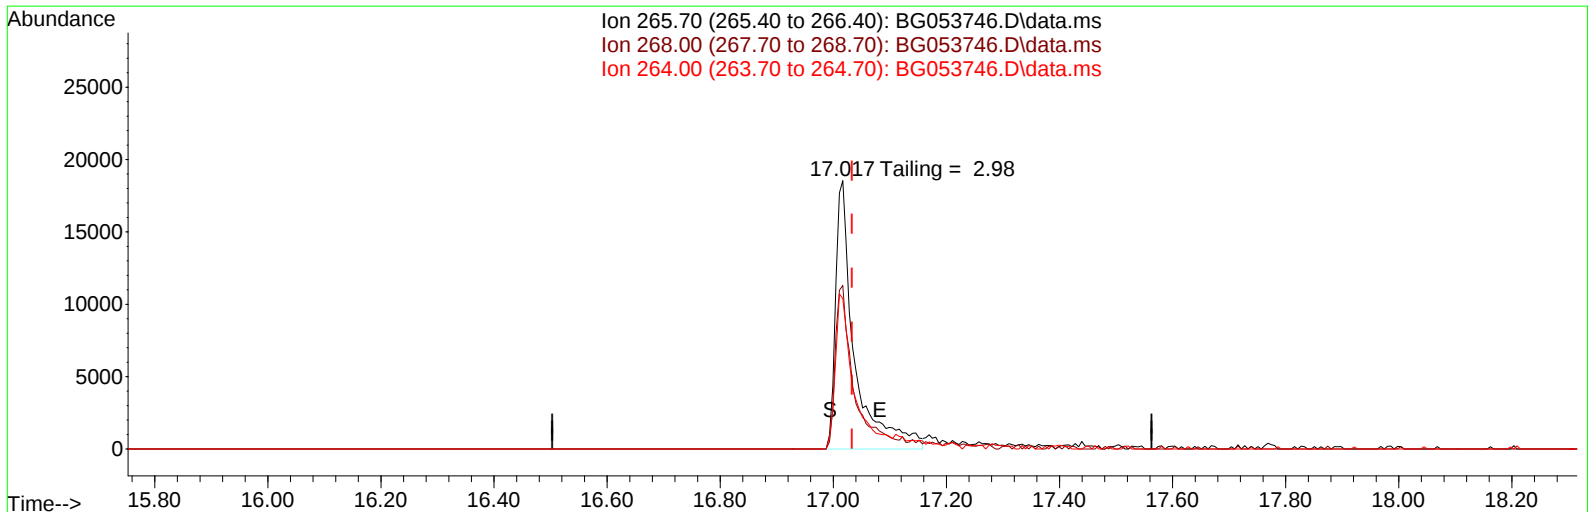

TIC: BG053746.D\data.ms

(70) Pentachlorophenol (C)

17.017min (-0.016) 27167.97 ng




response 42114

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	60.95
264.00	66.20	56.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052822\
Data File : BG053746.D
Acq On : 28 May 2022 10:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 28 11:04:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 15:11:41 2022
Response via : Initial Calibration

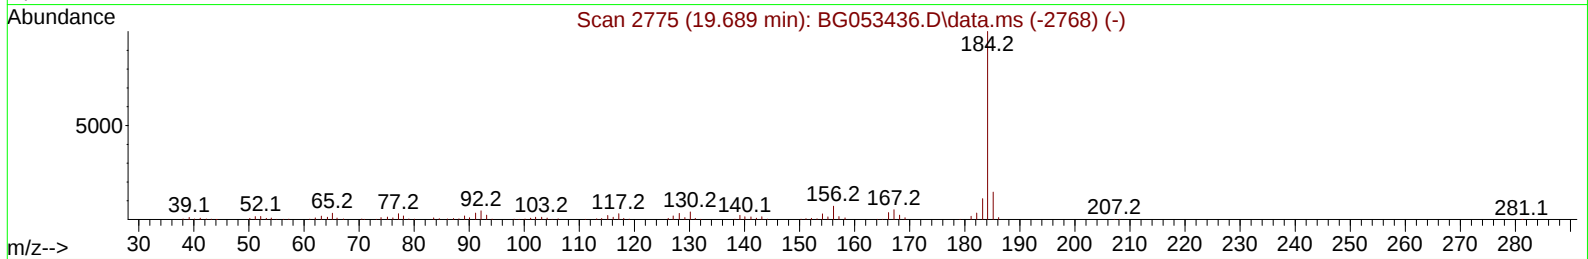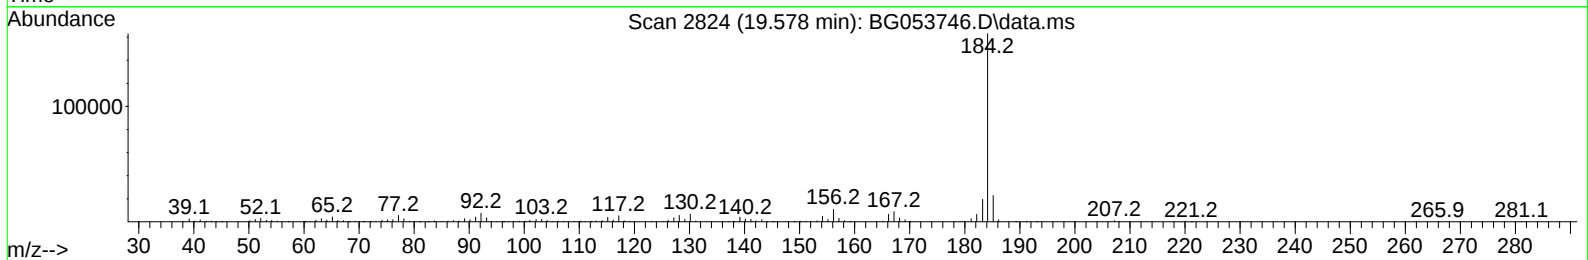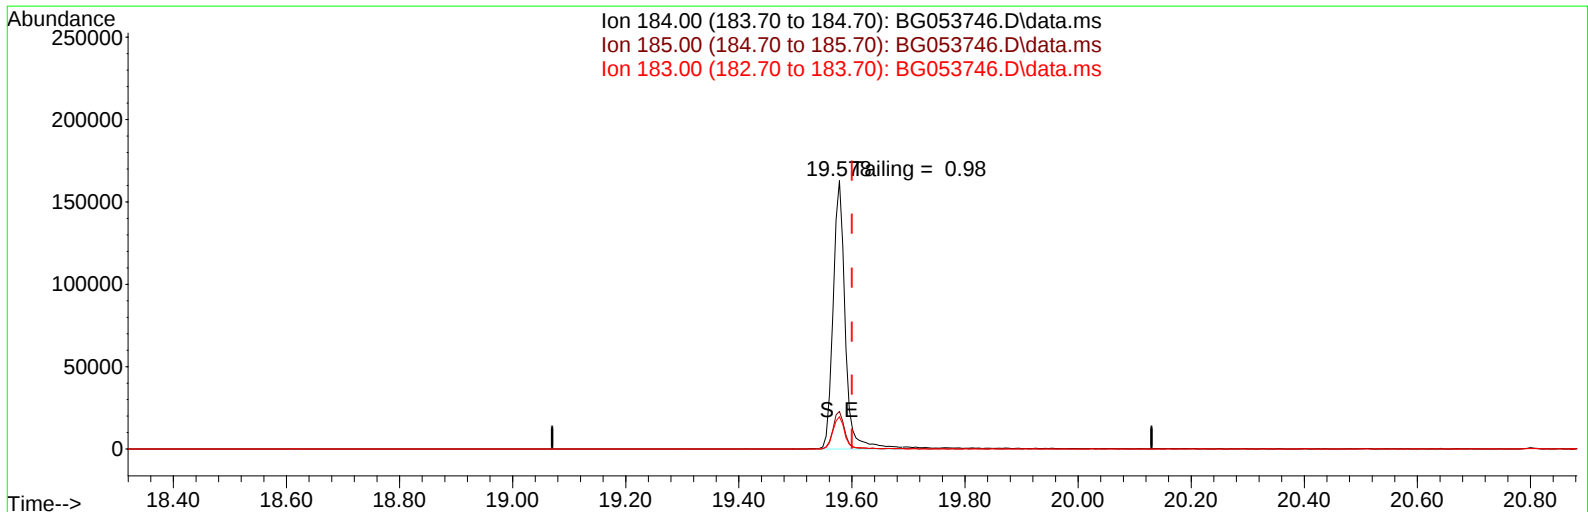

TIC: BG053746.D\data.ms

(77) Benzidine

19.578min (-0.022) 5616.57 ng

response 242842

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.01
183.00	11.10	12.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/28/2022	BNA_G	<u>BG053746.D</u>
Compound Name	Response	Retention Time
DDT	117334	20.8
DDD	2422	20.412
DDE	84	20.013
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2506	119840	2.09

Instrument :
BNA_G
ClientSampleId :
DFTPP