
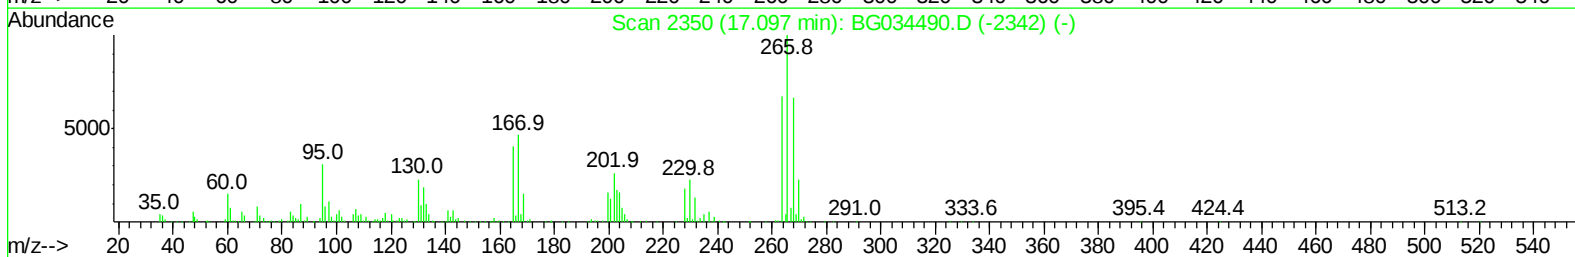
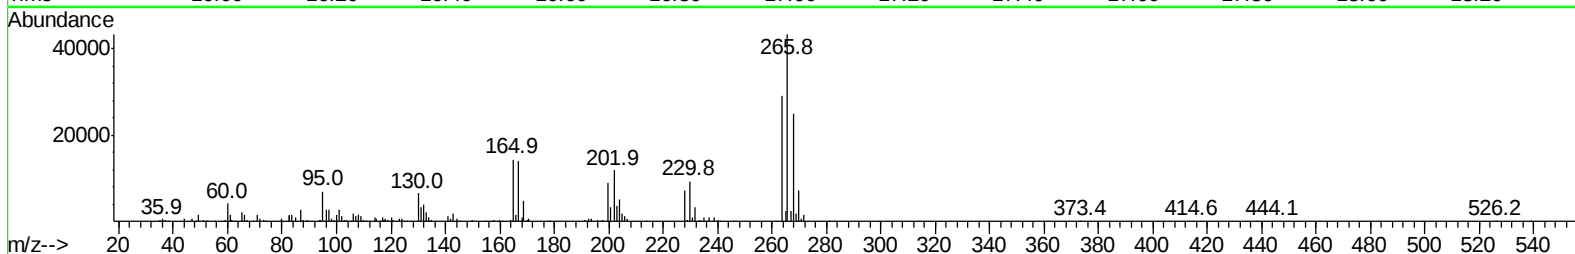


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG052918\  
Data File : BG034776.D  
Acq On : 29 May 2018 14:27  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 05:23:26 2018  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG051618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 25 14:58:34 2018  
Response via : Initial Calibration

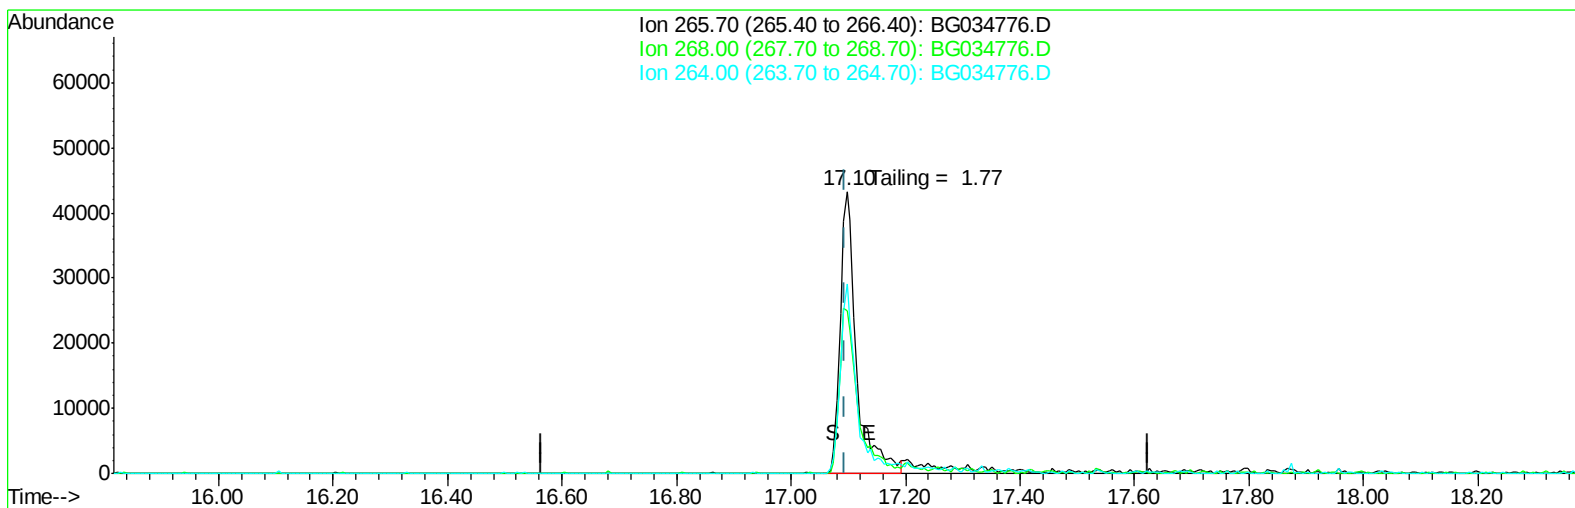

TIC: BG034776.D

(69) Pentachlorophenol (C)




17.098min (+0.003) 163988.73ng

response 86292

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 62.11 |
| 264.00 | 62.00 | 67.35 |
| 0.00   | 0.00  | 0.00  |

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG052918\  
Data File : BG034776.D  
Acq On : 29 May 2018 14:27  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 05:23:26 2018  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG051618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 25 14:58:34 2018  
Response via : Initial Calibration

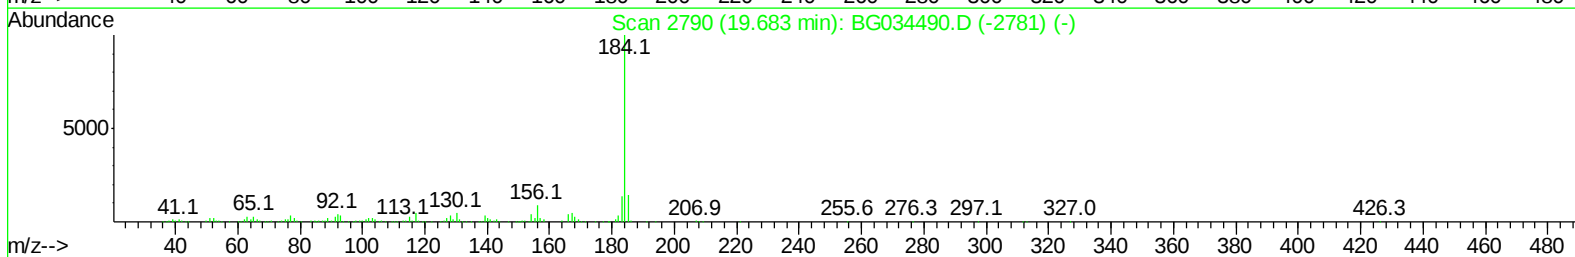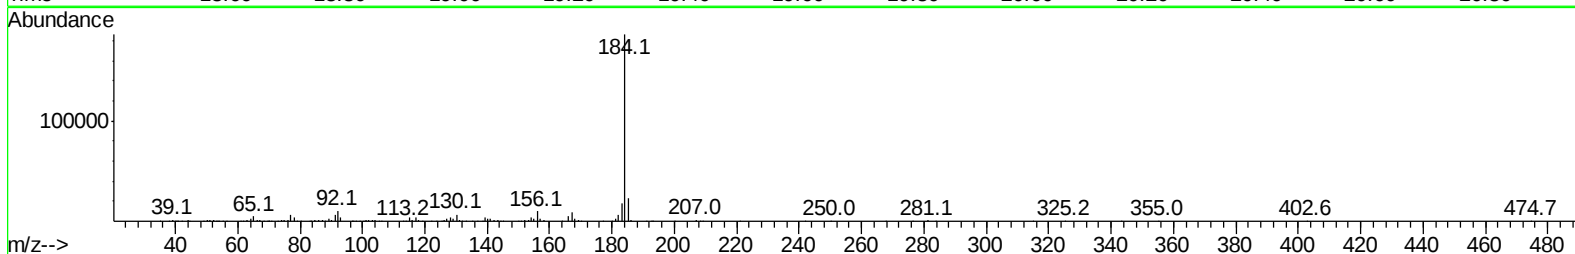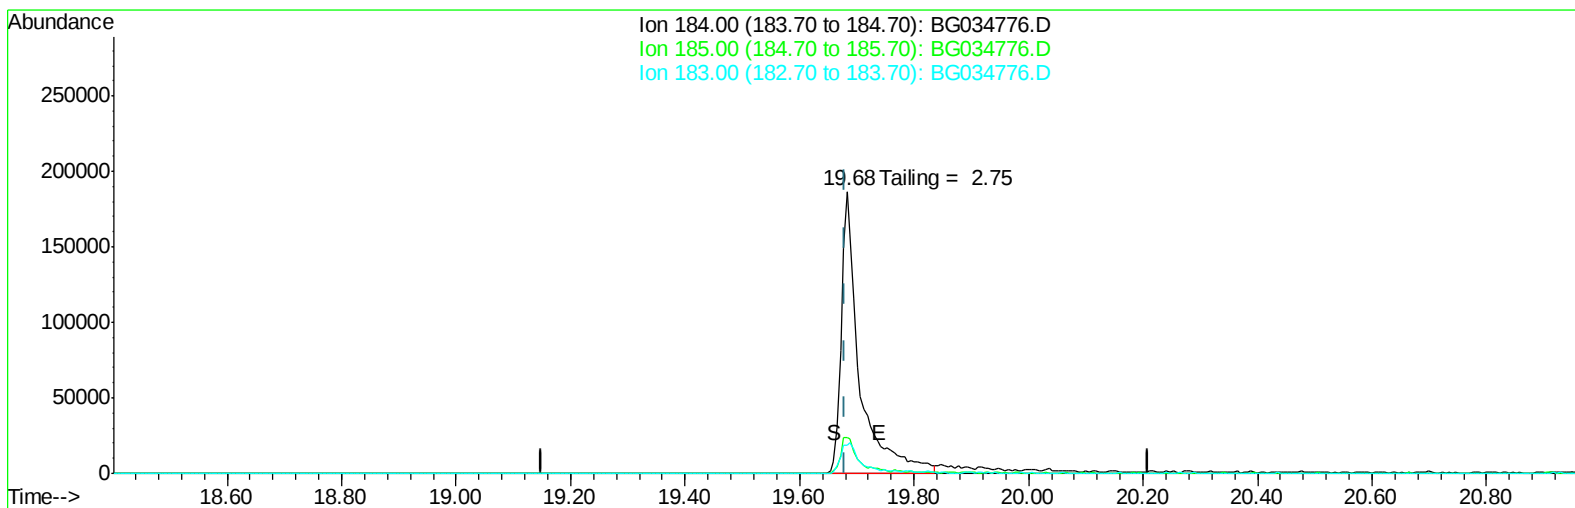

TIC: BG034776.D

(76) Benzidine

19.683min (+0.003) 248367.10ng

response 419686

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 12.73 |
| 183.00 | 13.30 | 9.92# |
| 0.00   | 0.00  | 0.00  |