
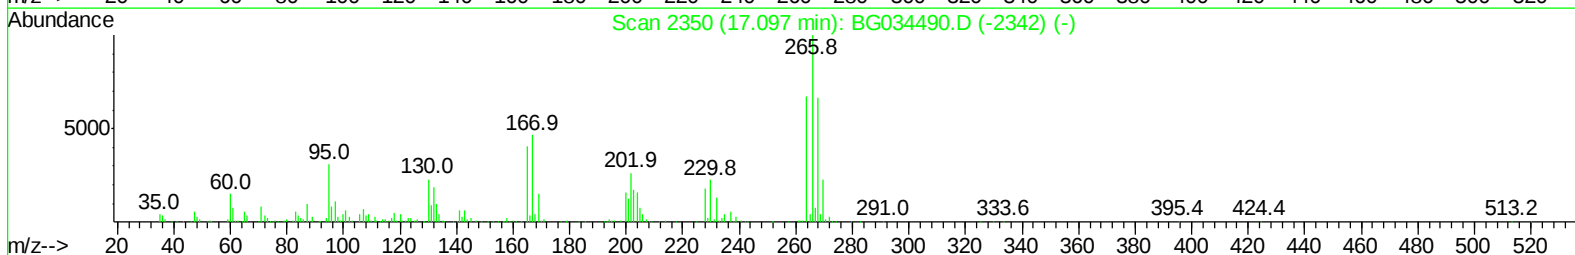
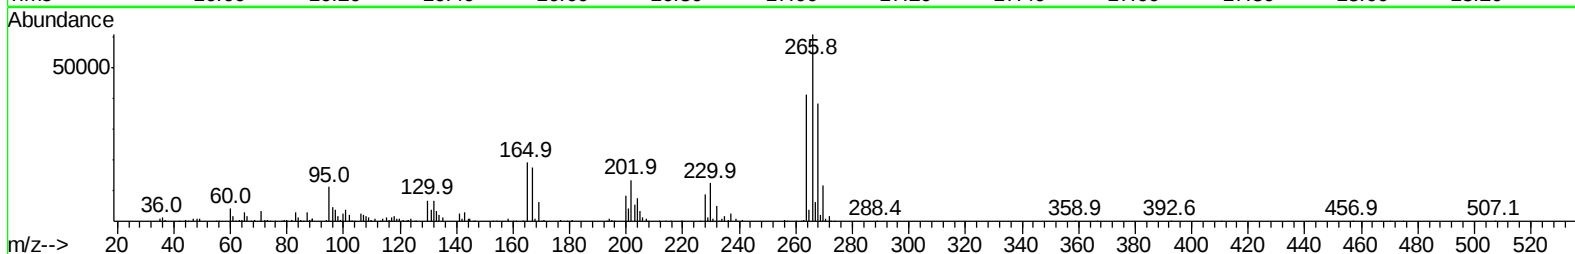


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG052918\
Data File : BG034795.D
Acq On : 30 May 2018 3:18
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 05:24:51 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG051618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 25 14:58:34 2018
Response via : Initial Calibration

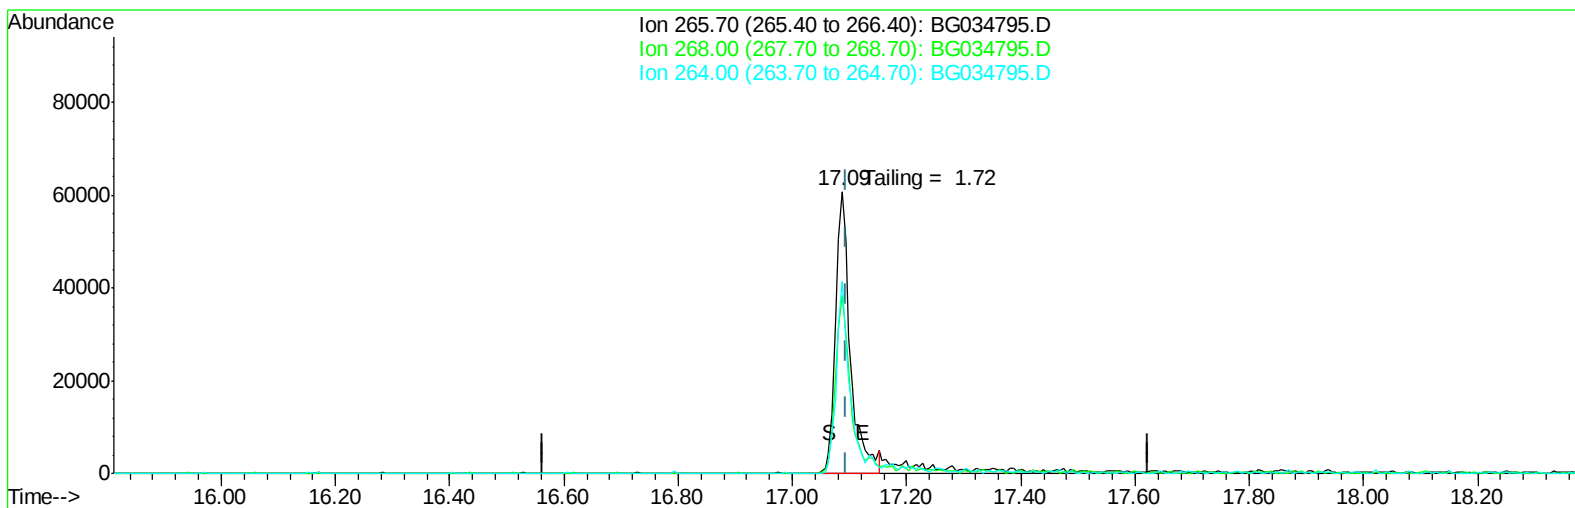

TIC: BG034795.D

(69) Pentachlorophenol (C)




17.087min (-0.008) 65331.88ng

response 107718

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.36
264.00	62.00	67.98
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG052918\
Data File : BG034795.D
Acq On : 30 May 2018 3:18
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 05:24:51 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG051618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 25 14:58:34 2018
Response via : Initial Calibration

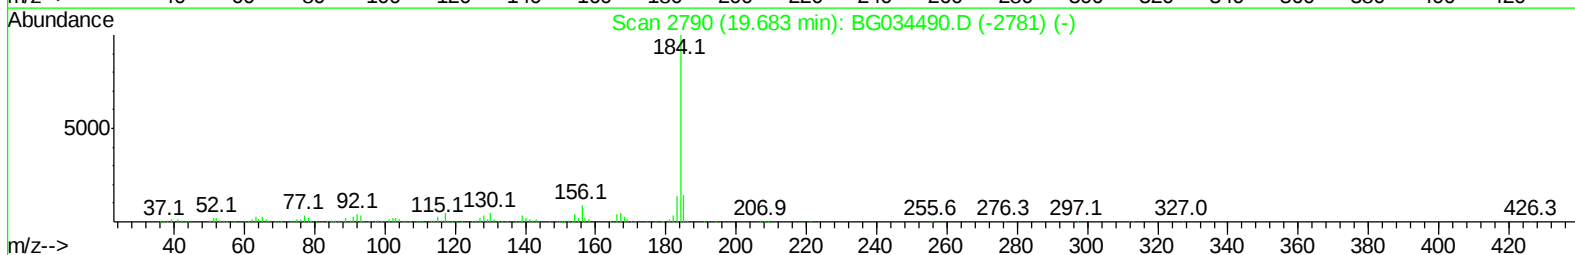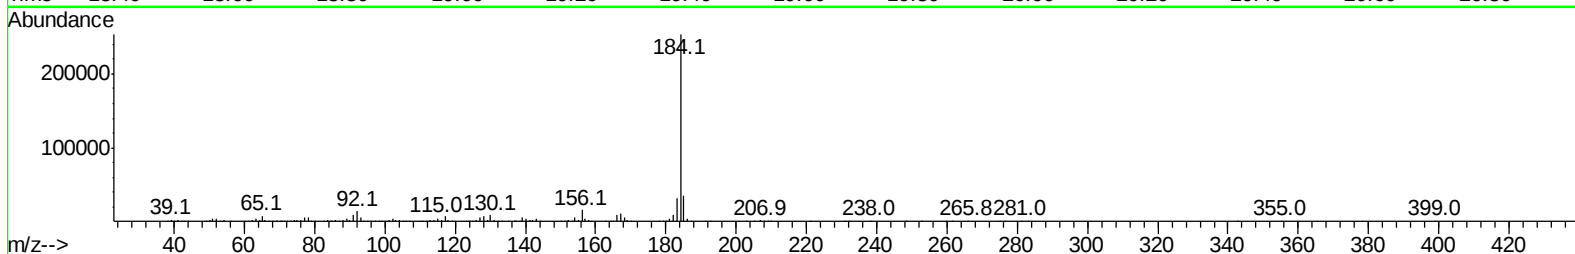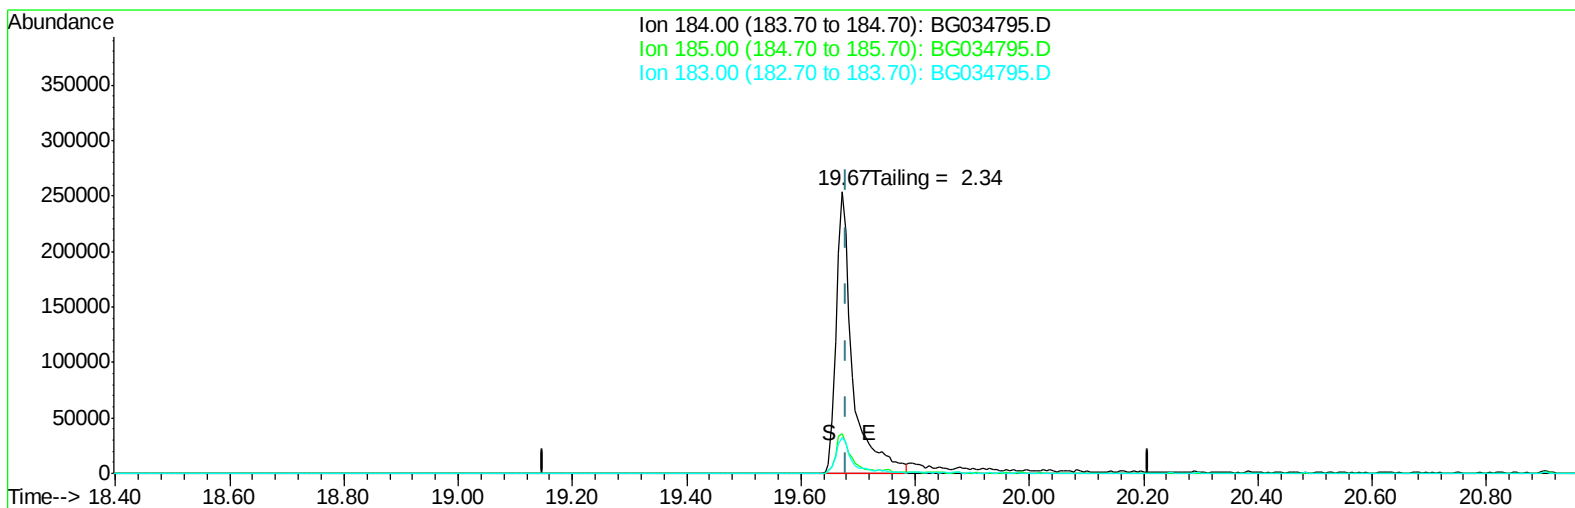

TIC: BG034795.D

(76) Benzidine

19.672min (-0.008) 74605.11ng

response 504249

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.08
183.00	13.30	12.73
0.00	0.00	0.00