

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052918\
 Data File : BG034784.D
 Acq On : 29 May 2018 19:36
 Operator : SJ/JU
 Sample : PB109727TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: May 30 04:44:08 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG051618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 25 14:58:34 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	72821	20.00	ng	0.00
21) Naphthalene-d8	10.85	136	284785	20.00	ng	0.00
38) Acenaphthene-d10	14.68	164	192670	20.00	ng	0.00
63) Phenanthrene-d10	17.43	188	515940	20.00	ng	0.00
75) Chrysene-d12	21.72	240	634348	20.00	ng	-0.02
86) Perylene-d12	24.98	264	644309	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	697743	147.58	ng	0.00
7) Phenol-d6	7.20	99	963075	125.92	ng	0.00
23) Nitrobenzene-d5	9.20	82	579587	77.74	ng	0.00
41) 2,4,6-Tribromophenol	16.17	330	444126	133.84	ng	0.00
44) 2-Fluorobiphenyl	13.30	172	1250761	88.13	ng	0.00
78) Terphenyl-d14	20.05	244	2564693	88.66	ng	0.00


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG052918\
Data File : BG034784.D
Acq On : 29 May 2018 19:36
Operator : SJ/JU
Sample : PB109727TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: May 30 04:44:08 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG051618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 25 14:58:34 2018
Response via : Initial Calibration

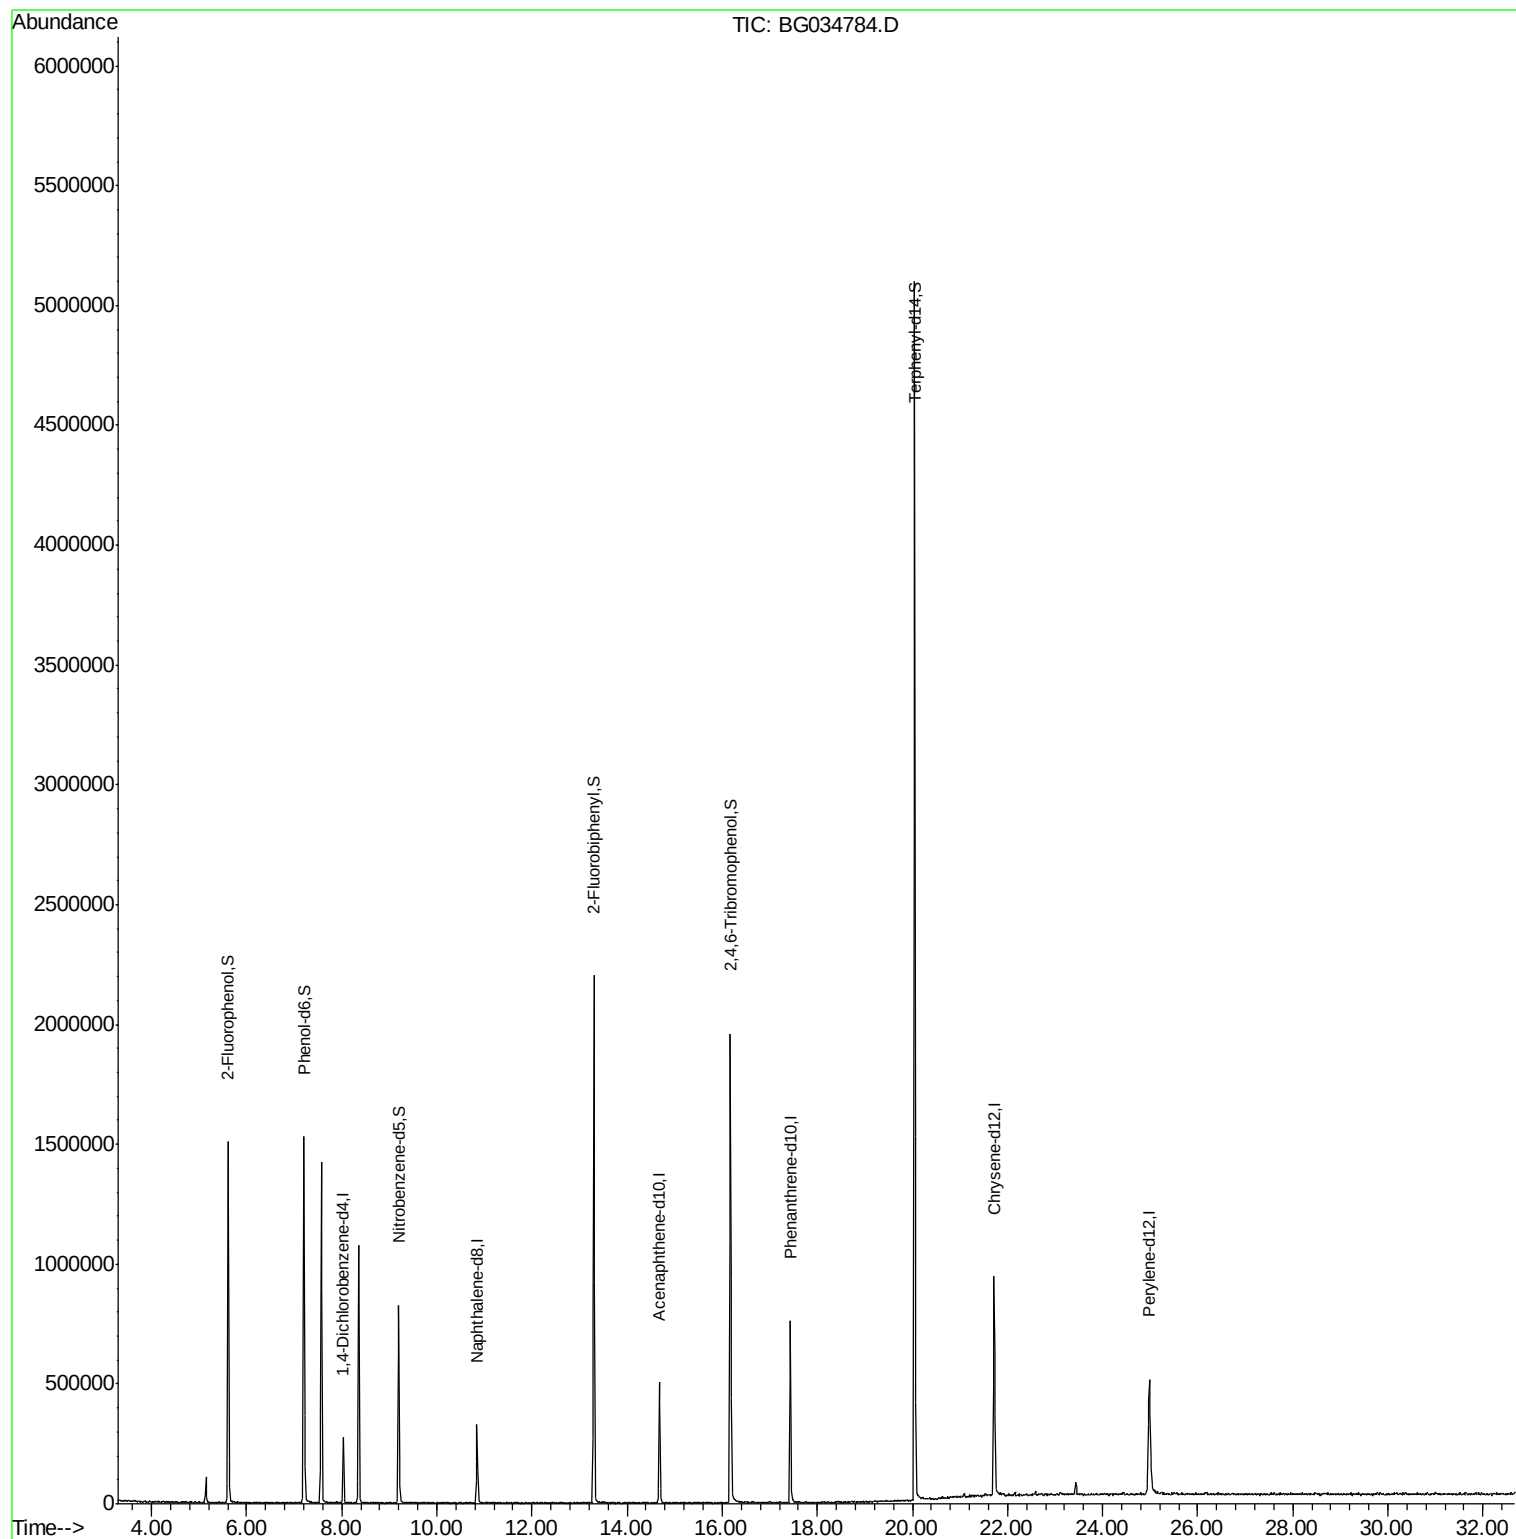


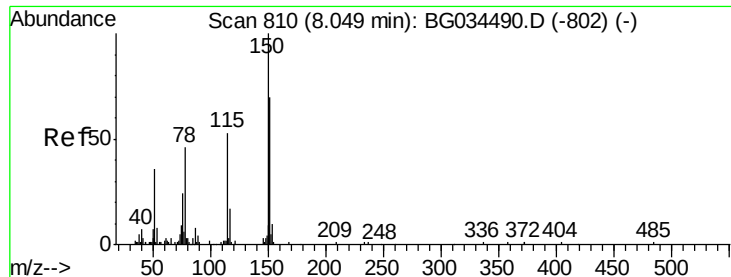

#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.03 min Scan# 807
Delta R.T. -0.00 min
Lab File: BG034784.D
Acq: 29 May 2018 19:36

Tot Ion	Ratio	Lower	Upper
152	100		
150	160.9	126.6	189.8
115	67.0	53.0	79.4



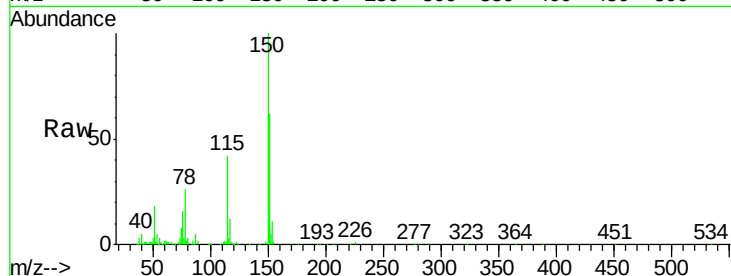


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

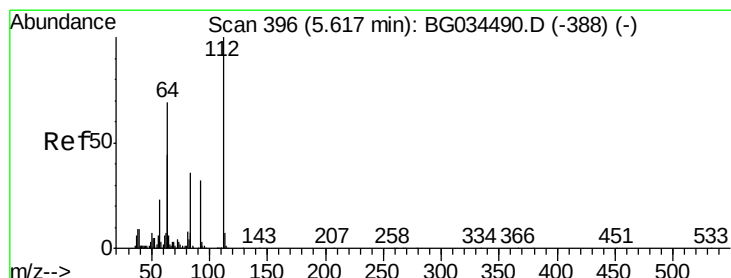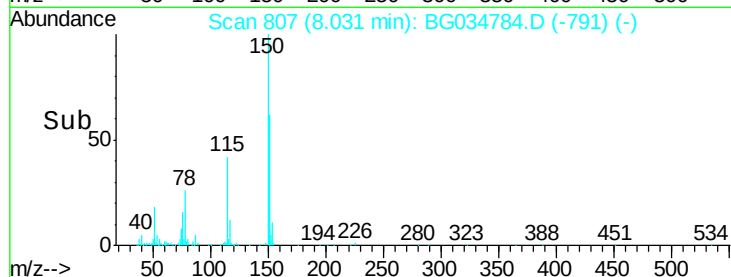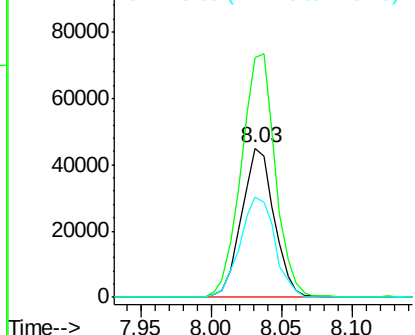

#5

2-Fluorophenol
Concen: 147.579 ng
RT: 5.61 min Scan# 395
Delta R.T. -0.00 min
Lab File: BG034784.D
Acq: 29 May 2018 19:36

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.4	56.3	84.5
63	29.8	30.1	45.1


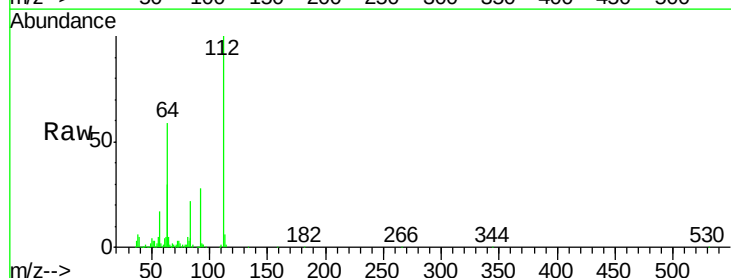



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

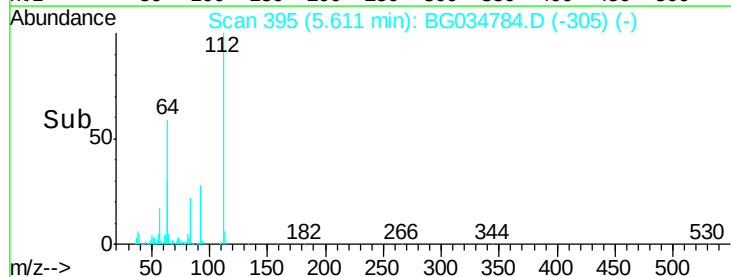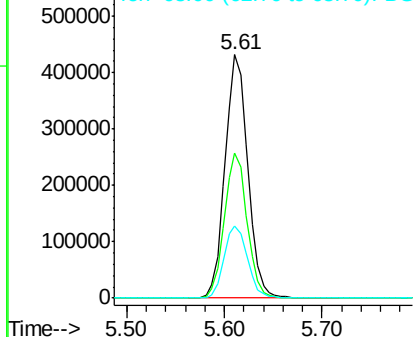

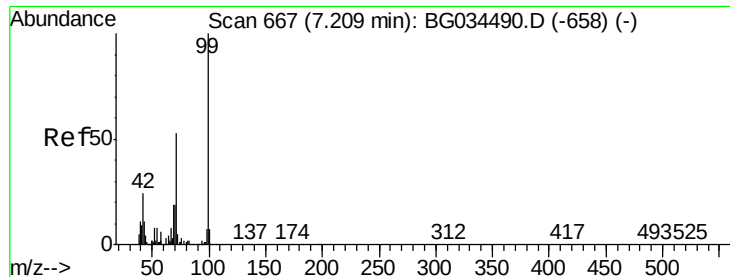

#7

Phenol-d6

Concen: 125.920 ng

RT: 7.20 min Scan# 666

Delta R.T. -0.00 min

Lab File: BG034784.D

Acq: 29 May 2018 19:36


Tot Ion: 99 Resp: 963075

Ion Ratio Lower Upper




99 100

42 14.1 14.1 21.1

71 38.4 26.1 39.1

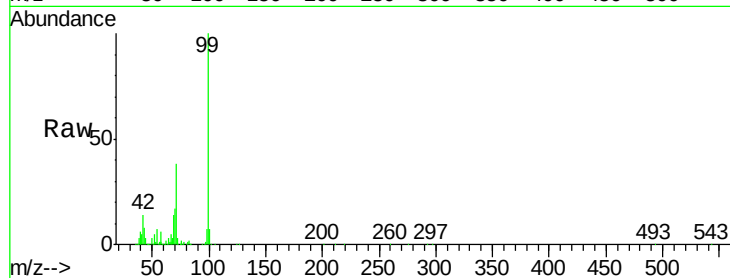

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

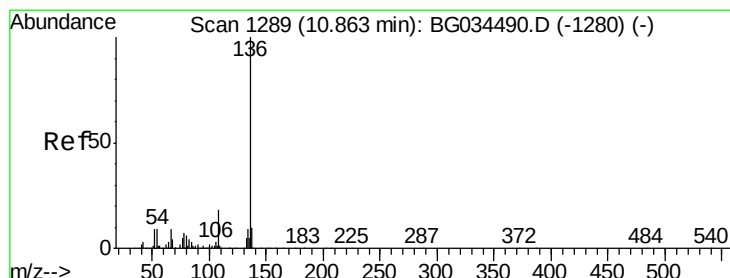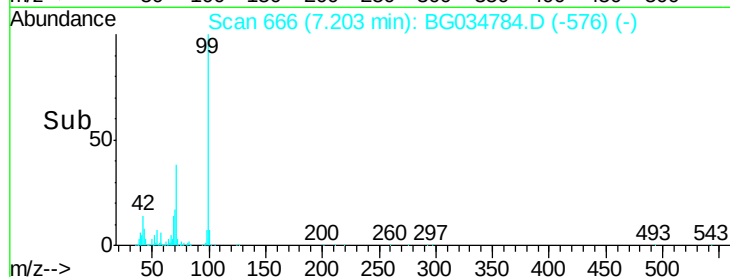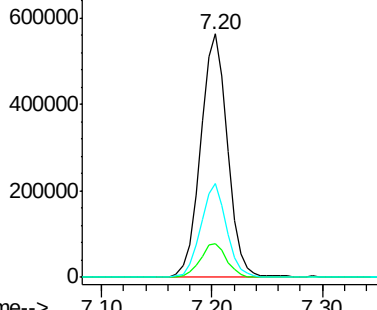

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1286

Delta R.T. -0.01 min

Lab File: BG034784.D

Acq: 29 May 2018 19:36

Tgt Ion: 136 Resp: 284785


Ion Ratio Lower Upper

136 100



137 11.7 9.2 13.8


54 7.8 10.3 15.5#

68 6.3 4.5 6.7

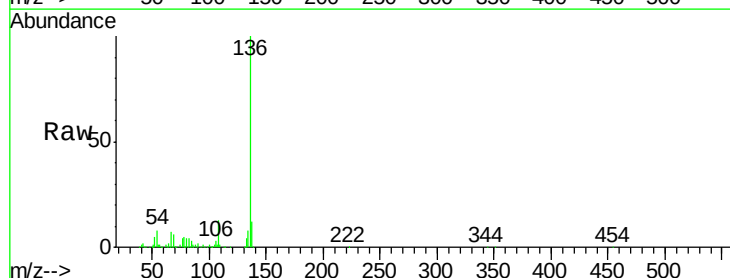





Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

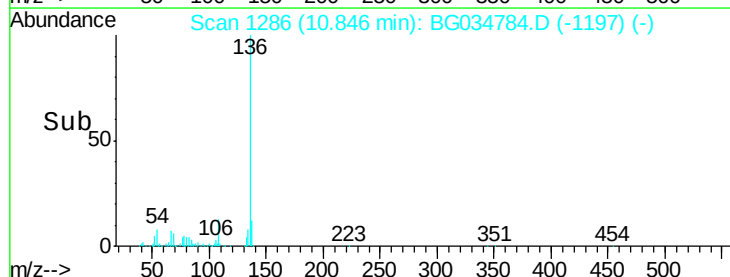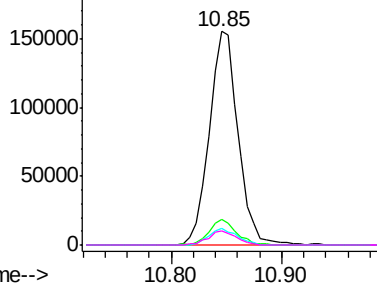

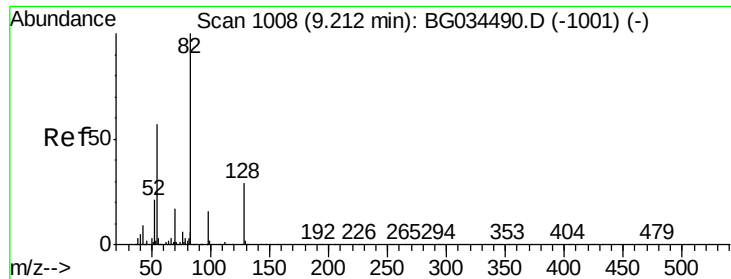




#23
 Nitrobenzene-d5
 Concen: 77.744 ng
 RT: 9.20 min Scan# 1006
 Delta R.T. -0.00 min
 Lab File: BG034784.D
 Acq: 29 May 2018 19:36


Tot Ion	82	Resp	579587
Ion Ratio	100	Lower	Upper
128	36.6	29.7	44.5
54	40.7	43.1	64.7#

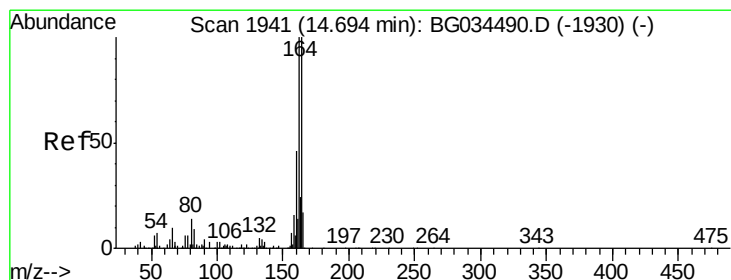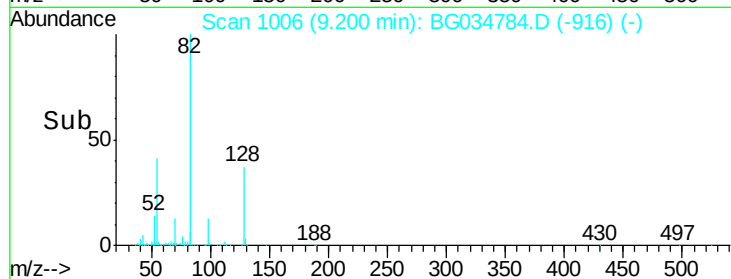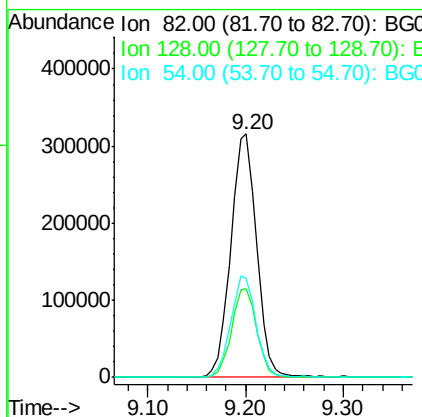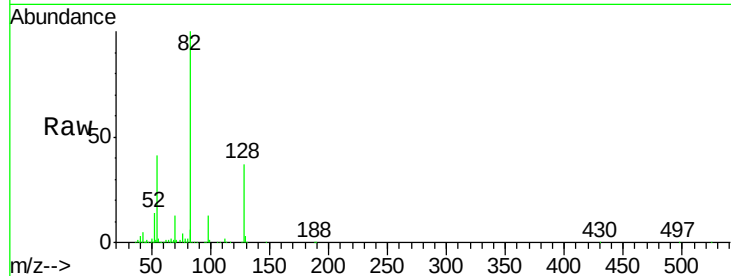

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.68 min Scan# 1939
 Delta R.T. -0.00 min
 Lab File: BG034784.D
 Acq: 29 May 2018 19:36


Tgt Ion	164	Resp	192670
Ion Ratio	100	Lower	Upper
162	101.1	78.8	118.2
160	42.7	35.4	53.0

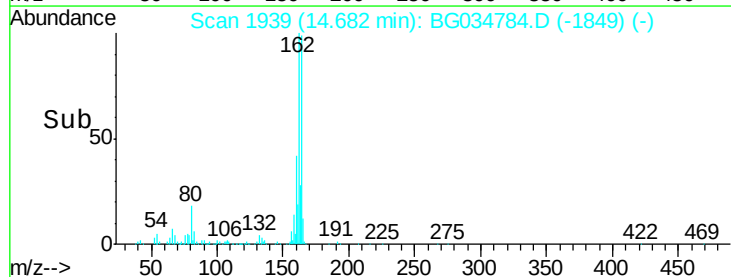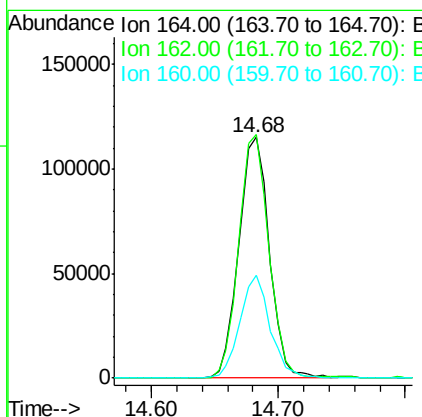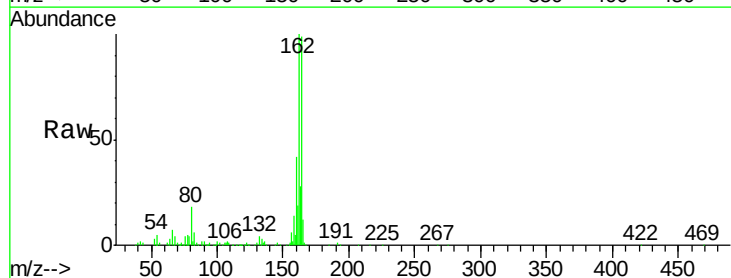



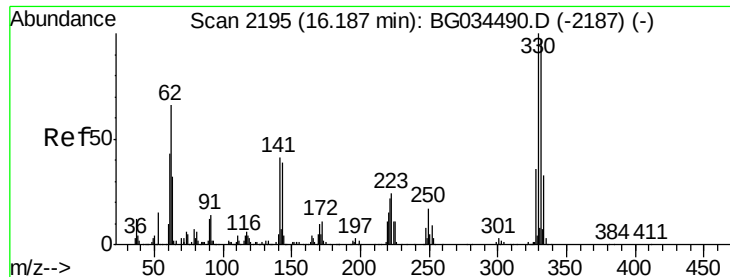


#41
 2,4,6-Tribromophenol
 Concen: 133.842 ng
 RT: 16.17 min Scan# 2193
 Delta R.T. -0.01 min
 Lab File: BG034784.D
 Acq: 29 May 2018 19:36

Tot Ion	Ratio	Lower	Upper
330	100		
332	98.6	77.0	115.6
141	27.5	25.2	37.8

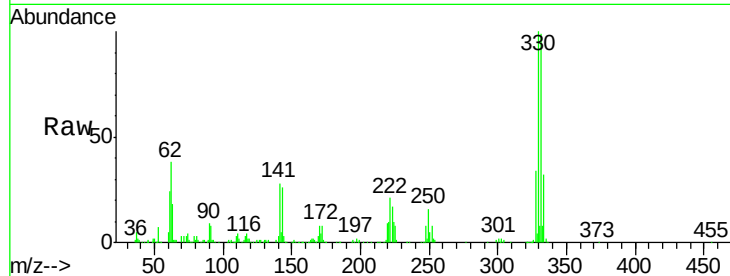


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

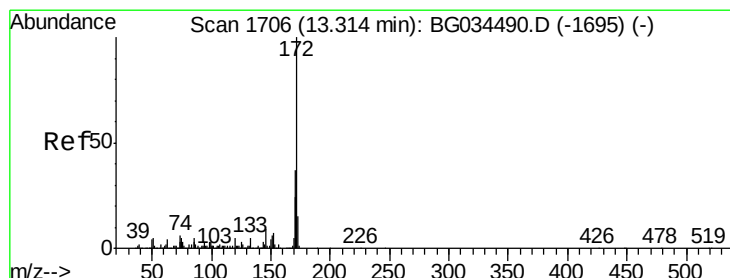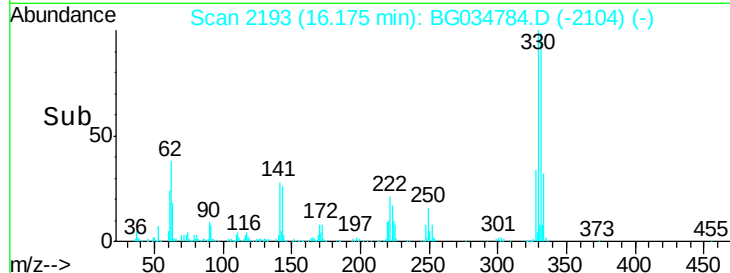
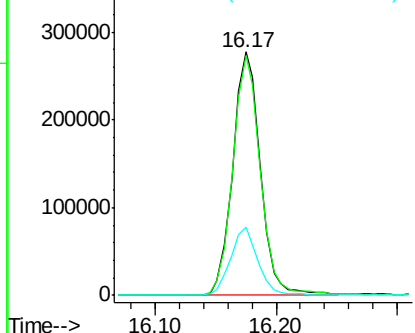



#44
 2-Fluorobiphenyl
 Concen: 88.133 ng
 RT: 13.30 min Scan# 1704
 Delta R.T. -0.00 min
 Lab File: BG034784.D
 Acq: 29 May 2018 19:36

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	30.0	45.0
170	23.2	19.5	29.3

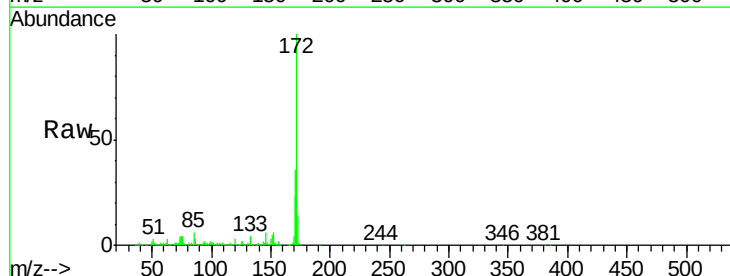

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

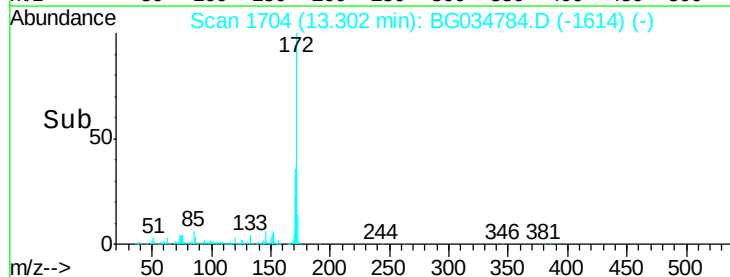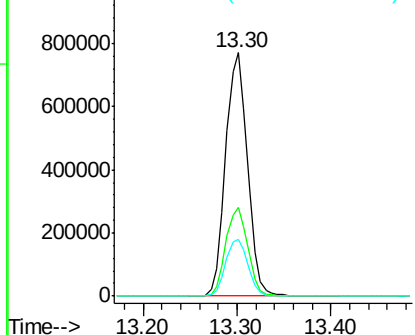

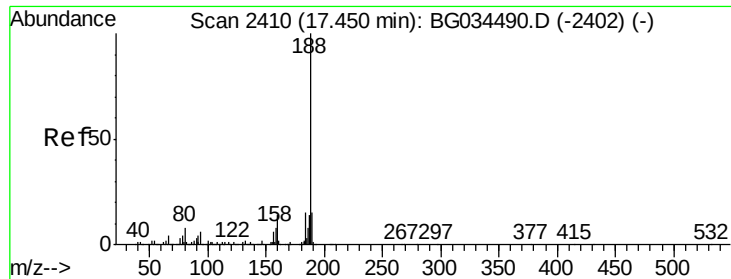

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.43 min Scan# 2407

Delta R.T. -0.01 min

Lab File: BG034784.D

Acq: 29 May 2018 19:36


Tot Ion:188 Resp: 515940

Ion Ratio Lower Upper

188 100

94 7.0 6.9 10.3




80 9.4 7.7 11.5

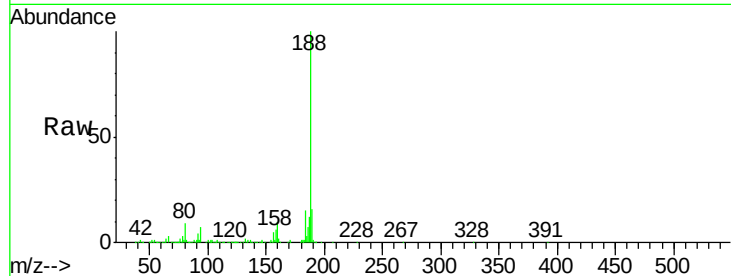

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG034784.D (-2407) (-)

Ion 80.00 (79.70 to 80.70): BG034784.D (-2407) (-)

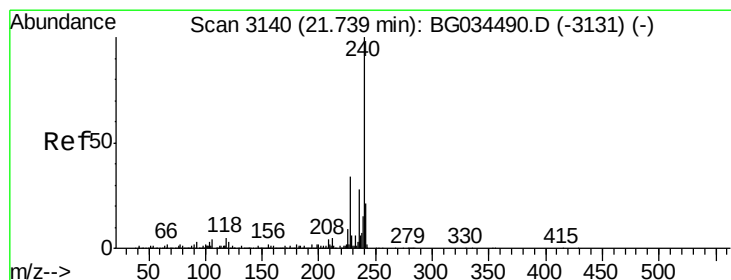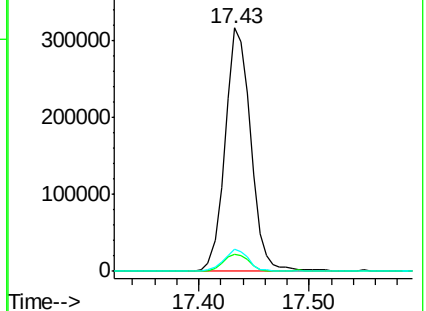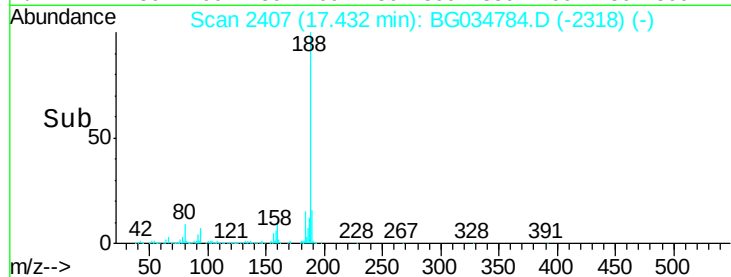

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.72 min Scan# 3137

Delta R.T. -0.02 min

Lab File: BG034784.D

Acq: 29 May 2018 19:36


Tgt Ion:240 Resp: 634348

Ion Ratio Lower Upper

240 100

120 6.6 6.8 10.2#



236 24.7 20.9 31.3

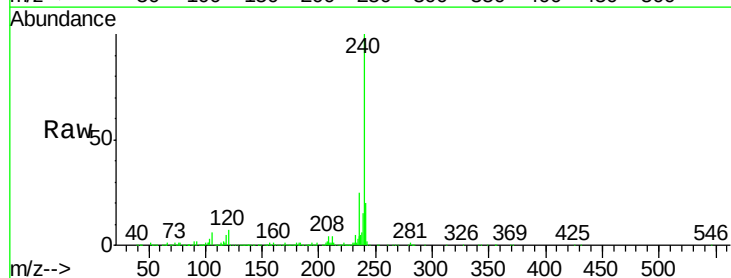


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

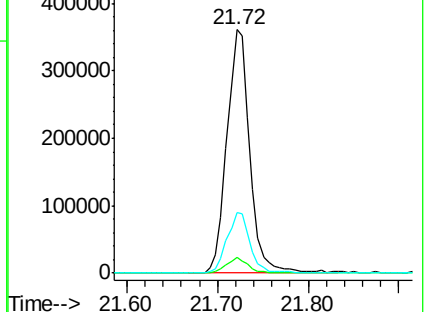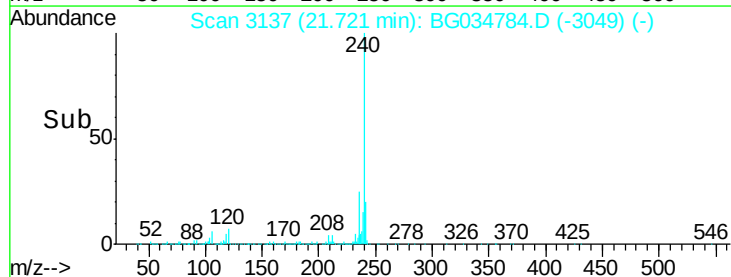

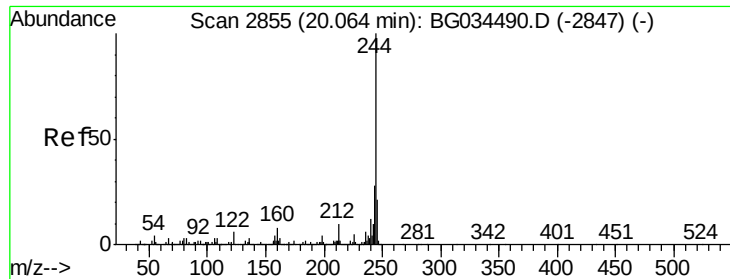

#78

Terphenyl-d14

Concen: 88.662 ng

RT: 20.05 min Scan# 2853

Delta R.T. -0.01 min

Lab File: BG034784.D

Acq: 29 May 2018 19:36


Tot Ion:244 Resp: 2564693

Ion Ratio Lower Upper




244 100

212 8.6 5.8 8.8

122 7.1 7.0 10.4

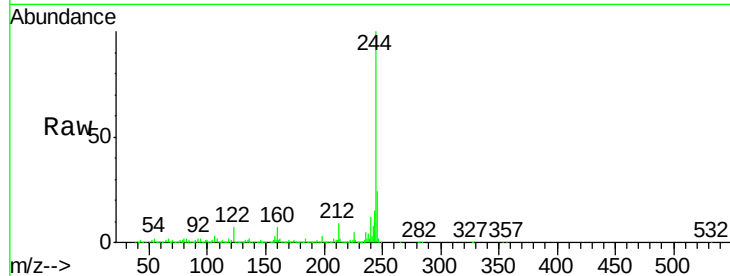

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

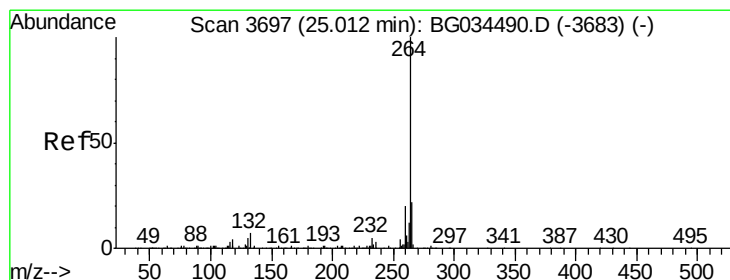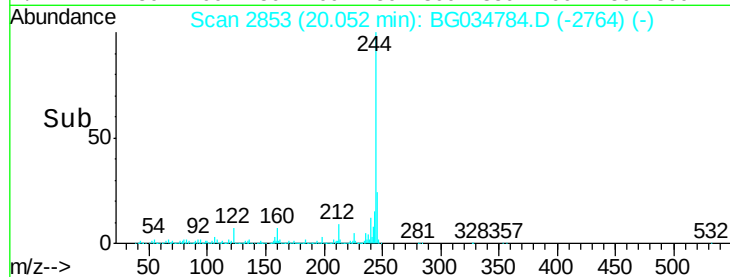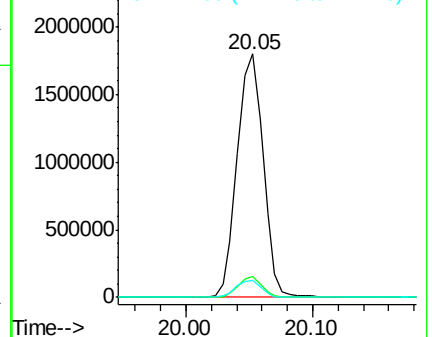

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.98 min Scan# 3692

Delta R.T. -0.02 min

Lab File: BG034784.D

Acq: 29 May 2018 19:36


Tgt Ion:264 Resp: 644309

Ion Ratio Lower Upper

264 100

260 23.0 17.4 26.0

265 20.6 17.7 26.5

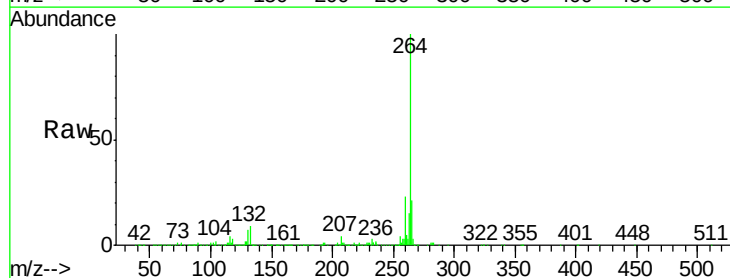

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

