


Data Path : Z:\HPCHEM1\BNA G\DATA\BG052918\
Data File : BG034776.D
Acq On : 29 May 2018 14:27
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051618.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 25 14:58:34 2018

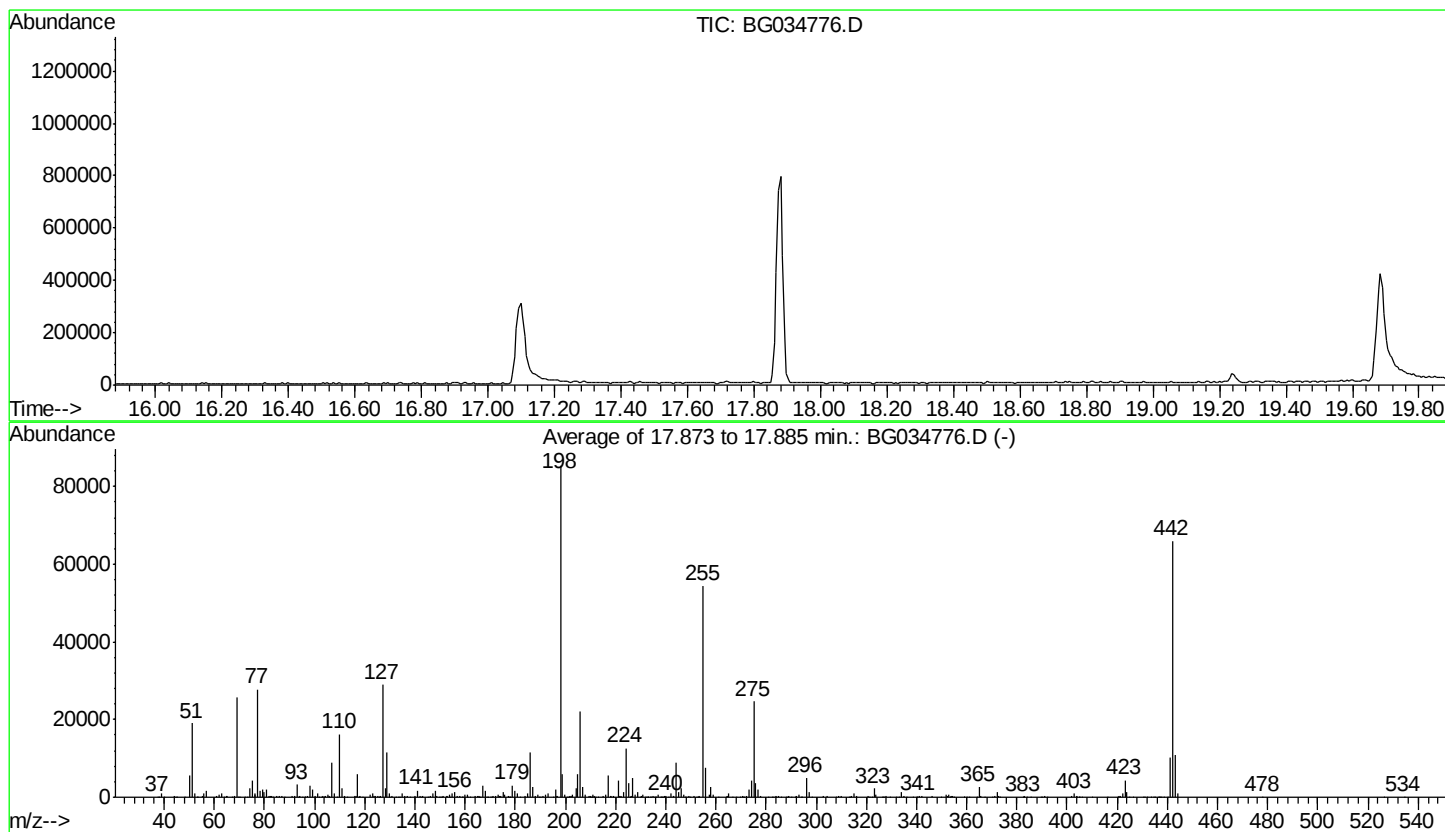

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.2	18958	PASS
68	69	0.00	2	1.7	441	PASS
69	198	0.00	100	30.3	25821	PASS
70	69	0.00	2	0.6	151	PASS
127	198	10	80	33.8	28850	PASS
197	198	0.00	2	0.6	470	PASS
198	198	100	100	100.0	85354	PASS
199	198	5	9	6.8	5786	PASS
275	198	10	60	28.9	24688	PASS
365	198	1	100	3.2	2754	PASS
441	443	0.01	100	94.3	10285	PASS
442	198	50	100	77.2	65909	PASS
443	442	15	24	16.5	10903	PASS