


Data Path : Z:\HPCHEM1\BNA G\DATA\BG052918\
 Data File : BG034795.D
 Acq On : 30 May 2018 3:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 25 14:58:34 2018

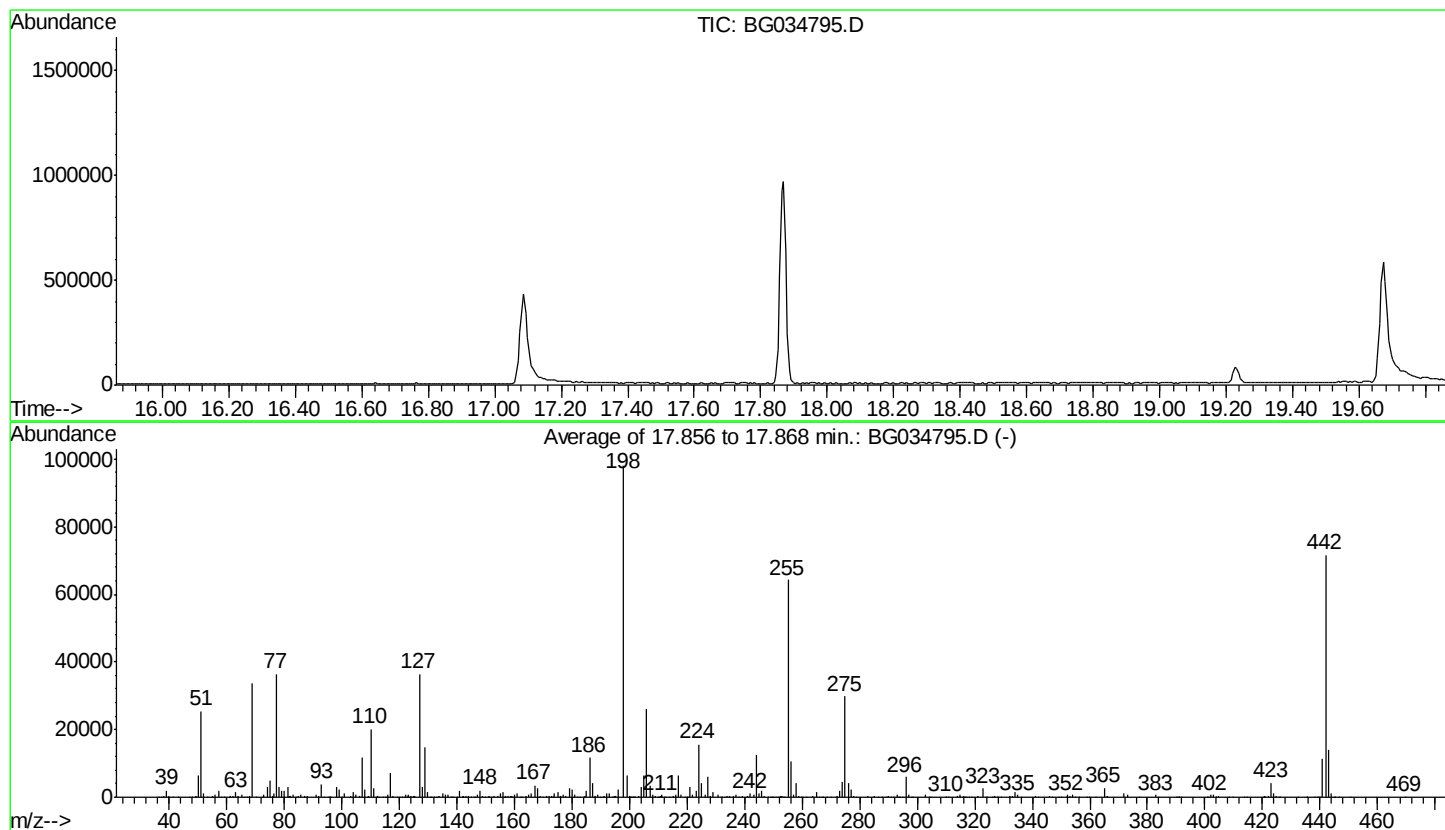

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.1	25552	PASS
68	69	0.00	2	0.6	205	PASS
69	198	0.00	100	34.5	33786	PASS
70	69	0.00	2	0.4	121	PASS
127	198	10	80	37.2	36469	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98053	PASS
199	198	5	9	6.7	6618	PASS
275	198	10	60	30.4	29808	PASS
365	198	1	100	2.7	2683	PASS
441	443	0.01	100	80.4	11380	PASS
442	198	50	100	73.1	71712	PASS
443	442	15	24	19.7	14162	PASS