



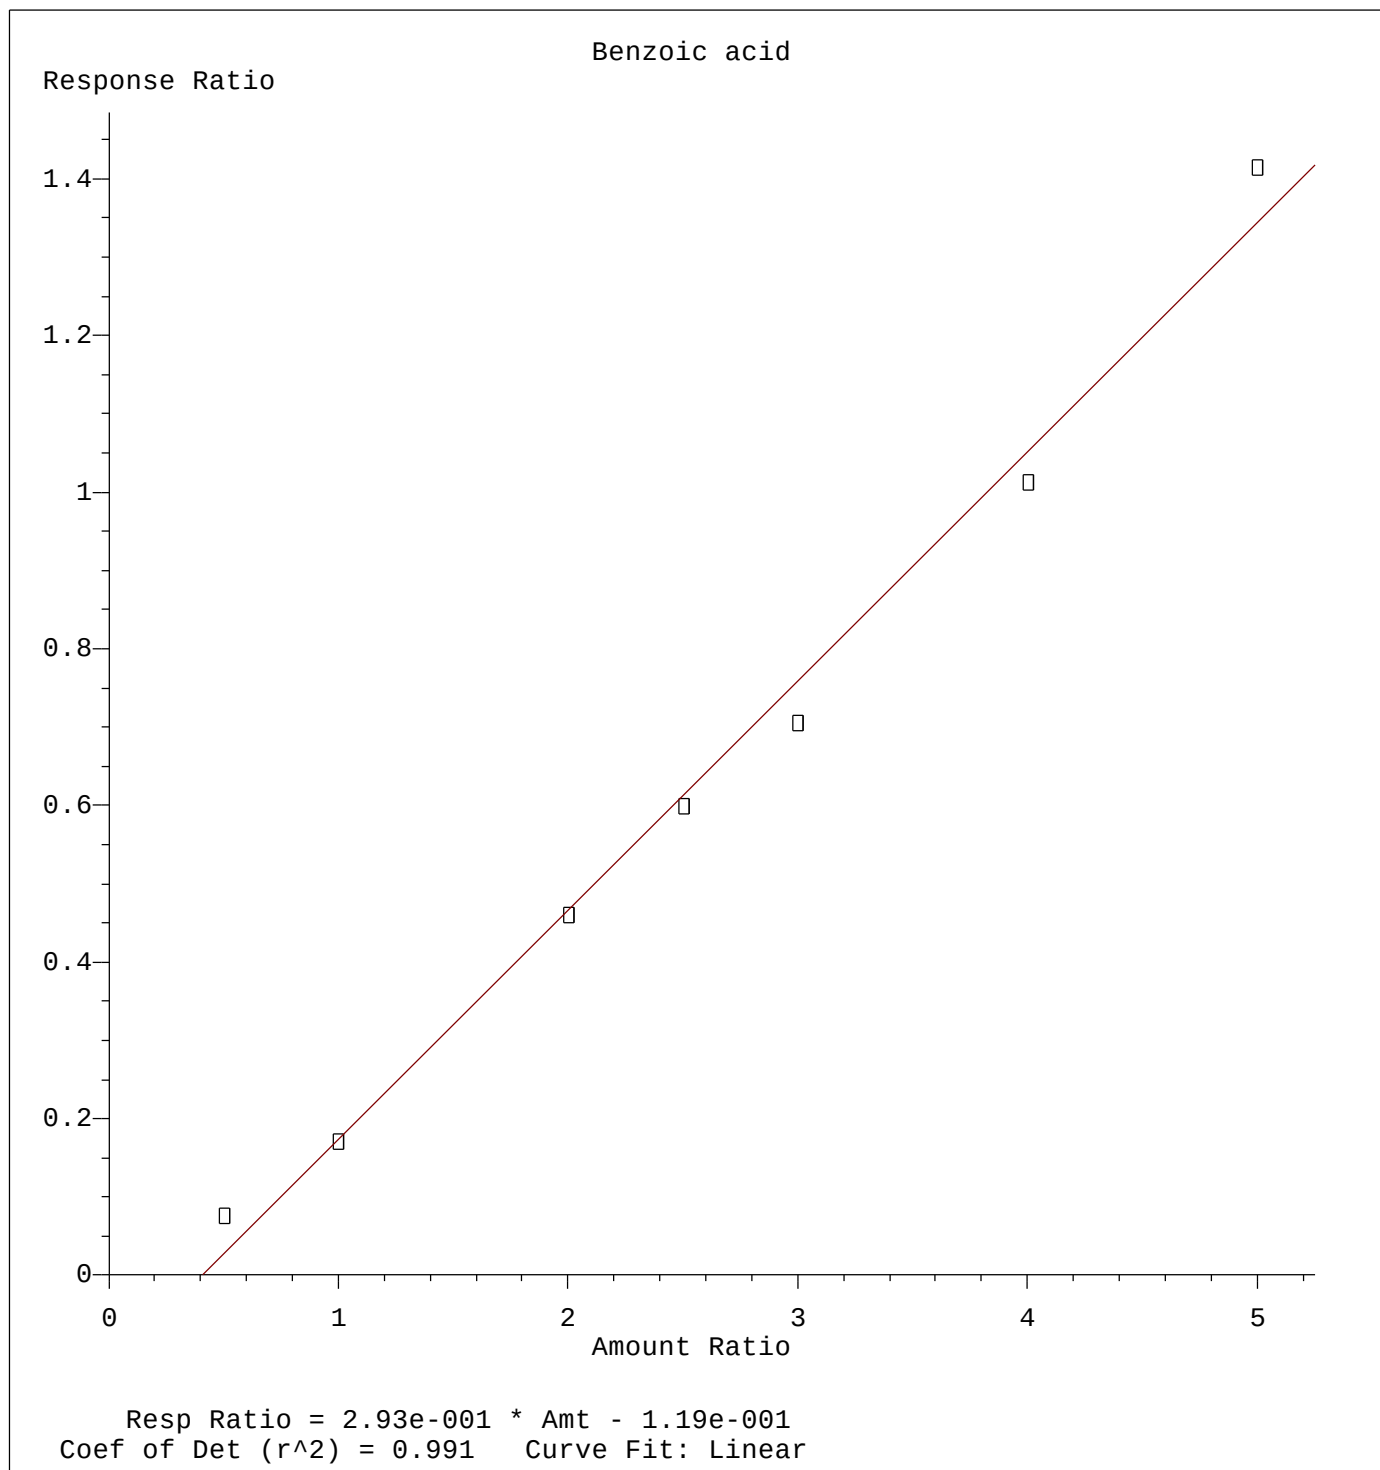

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
Calibration Table Last Updated: Wed May 29 18:39:57 2019

Hexachlorocyclopentadiene

Response Ratio

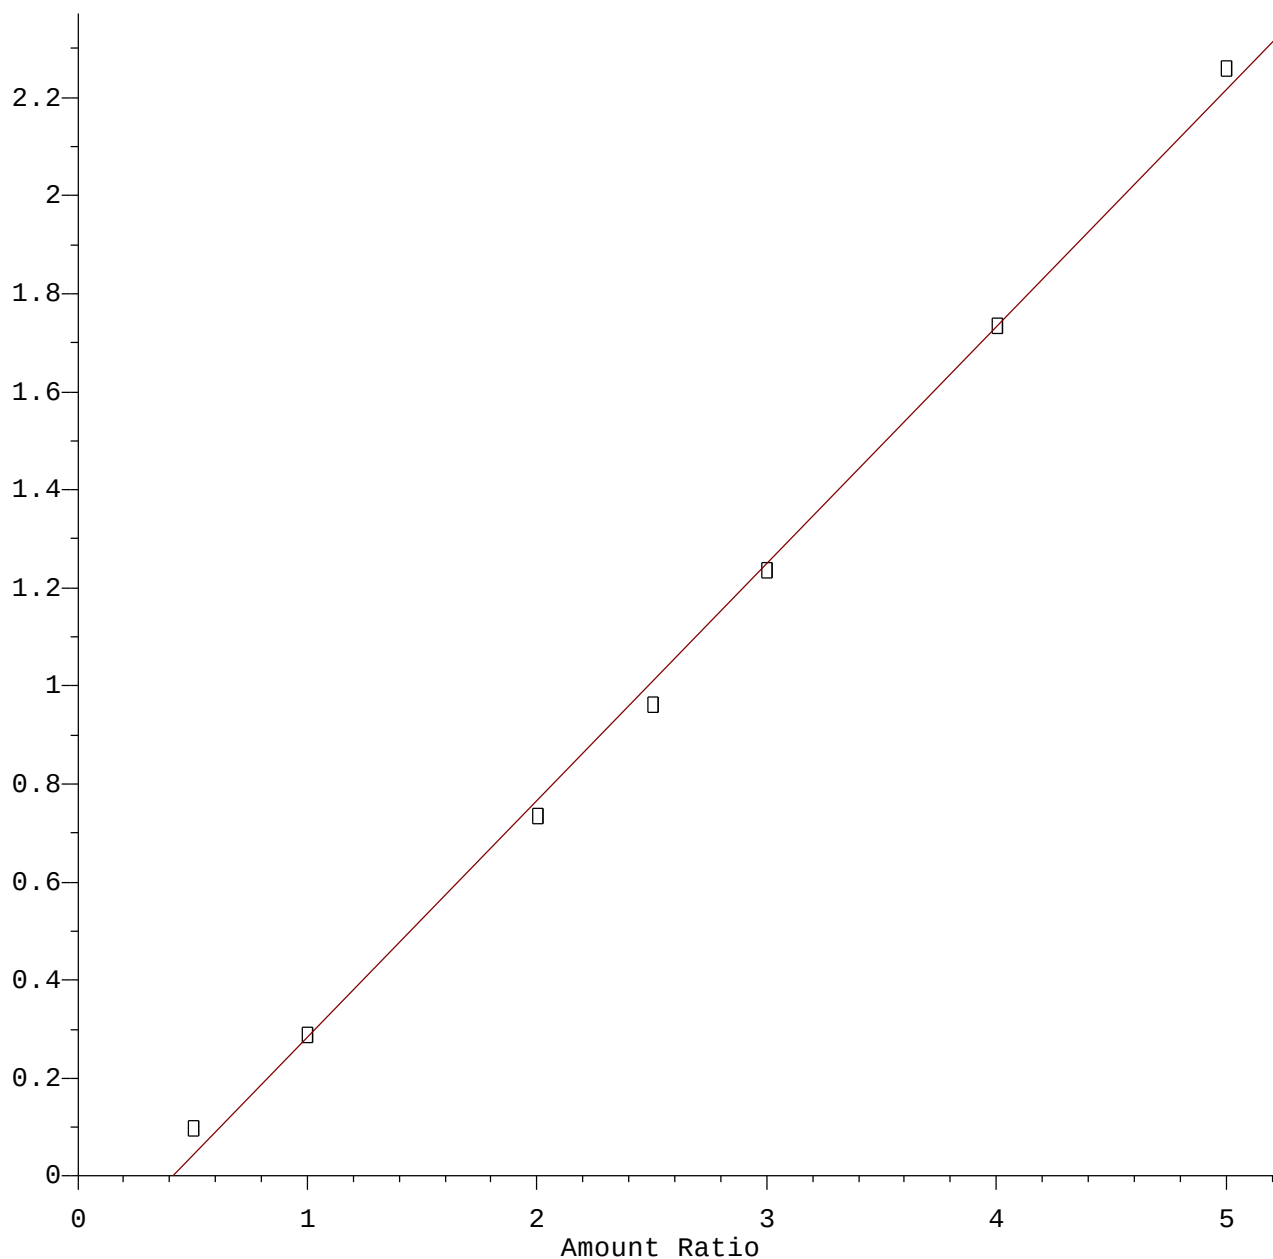


Resp Ratio = $4.83 \times 10^{-1} \times \text{Amt} - 1.99 \times 10^{-1}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
Calibration Table Last Updated: Wed May 29 18:39:57 2019

2,4-Dinitrophenol


Response Ratio

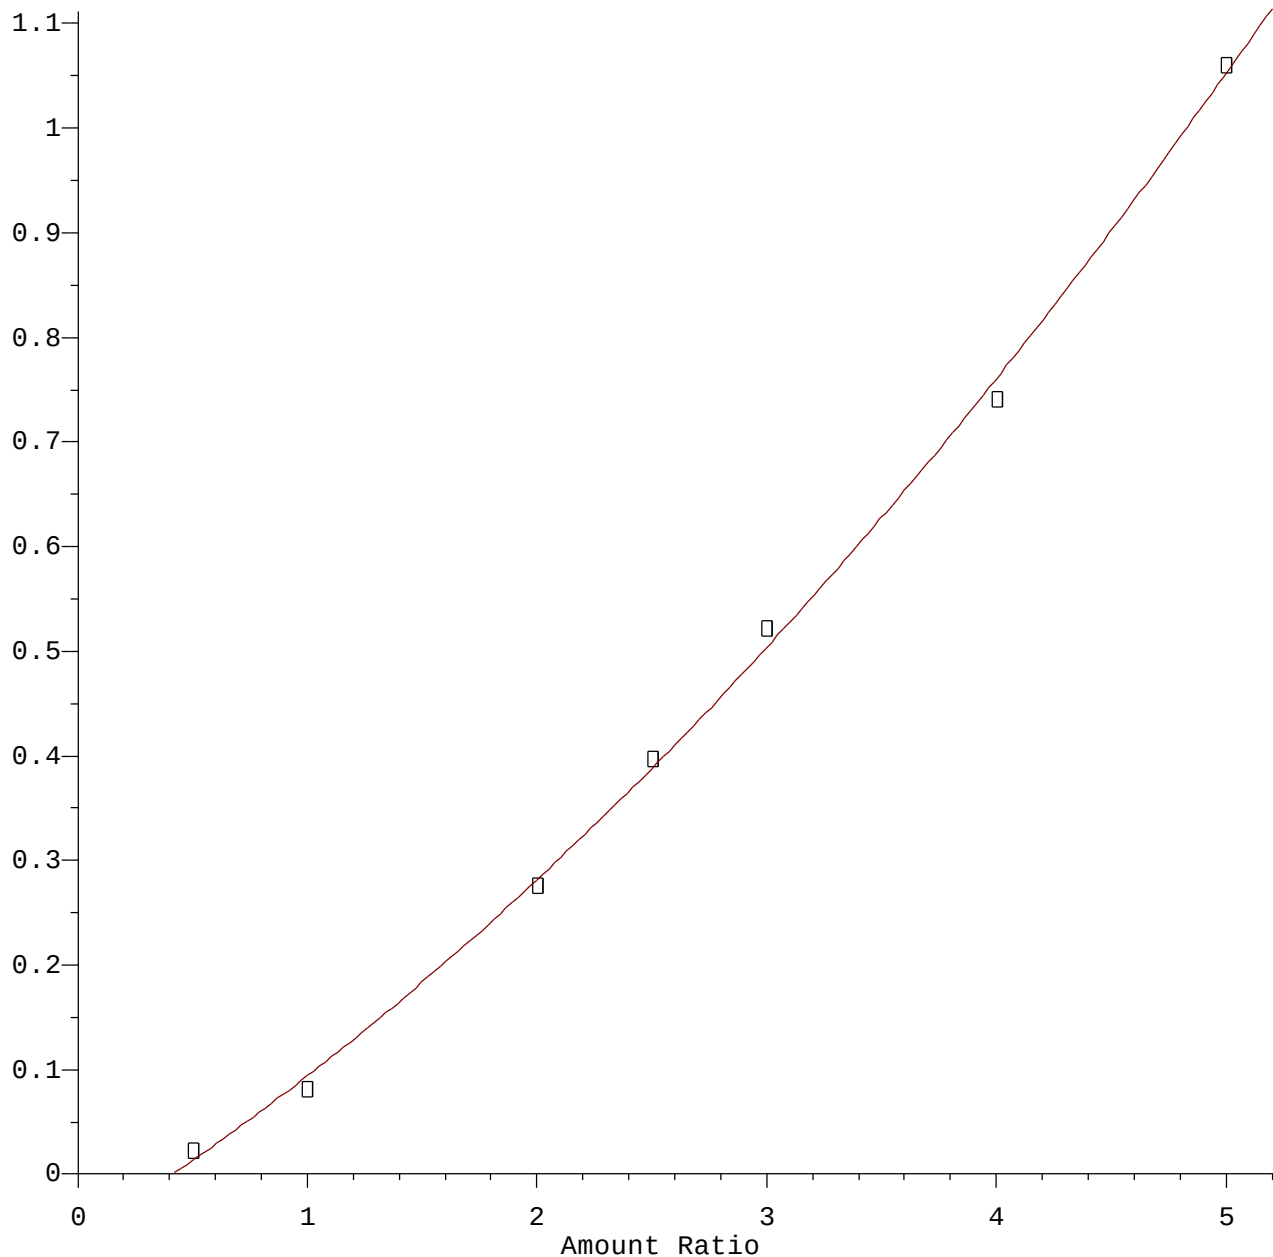

$R = 1.74e-002 A^2 + 1.35e-001 A - 5.88e-002$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic


Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
Calibration Table Last Updated: Wed May 29 18:39:57 2019

4,6-Dinitro-2-methylphenol

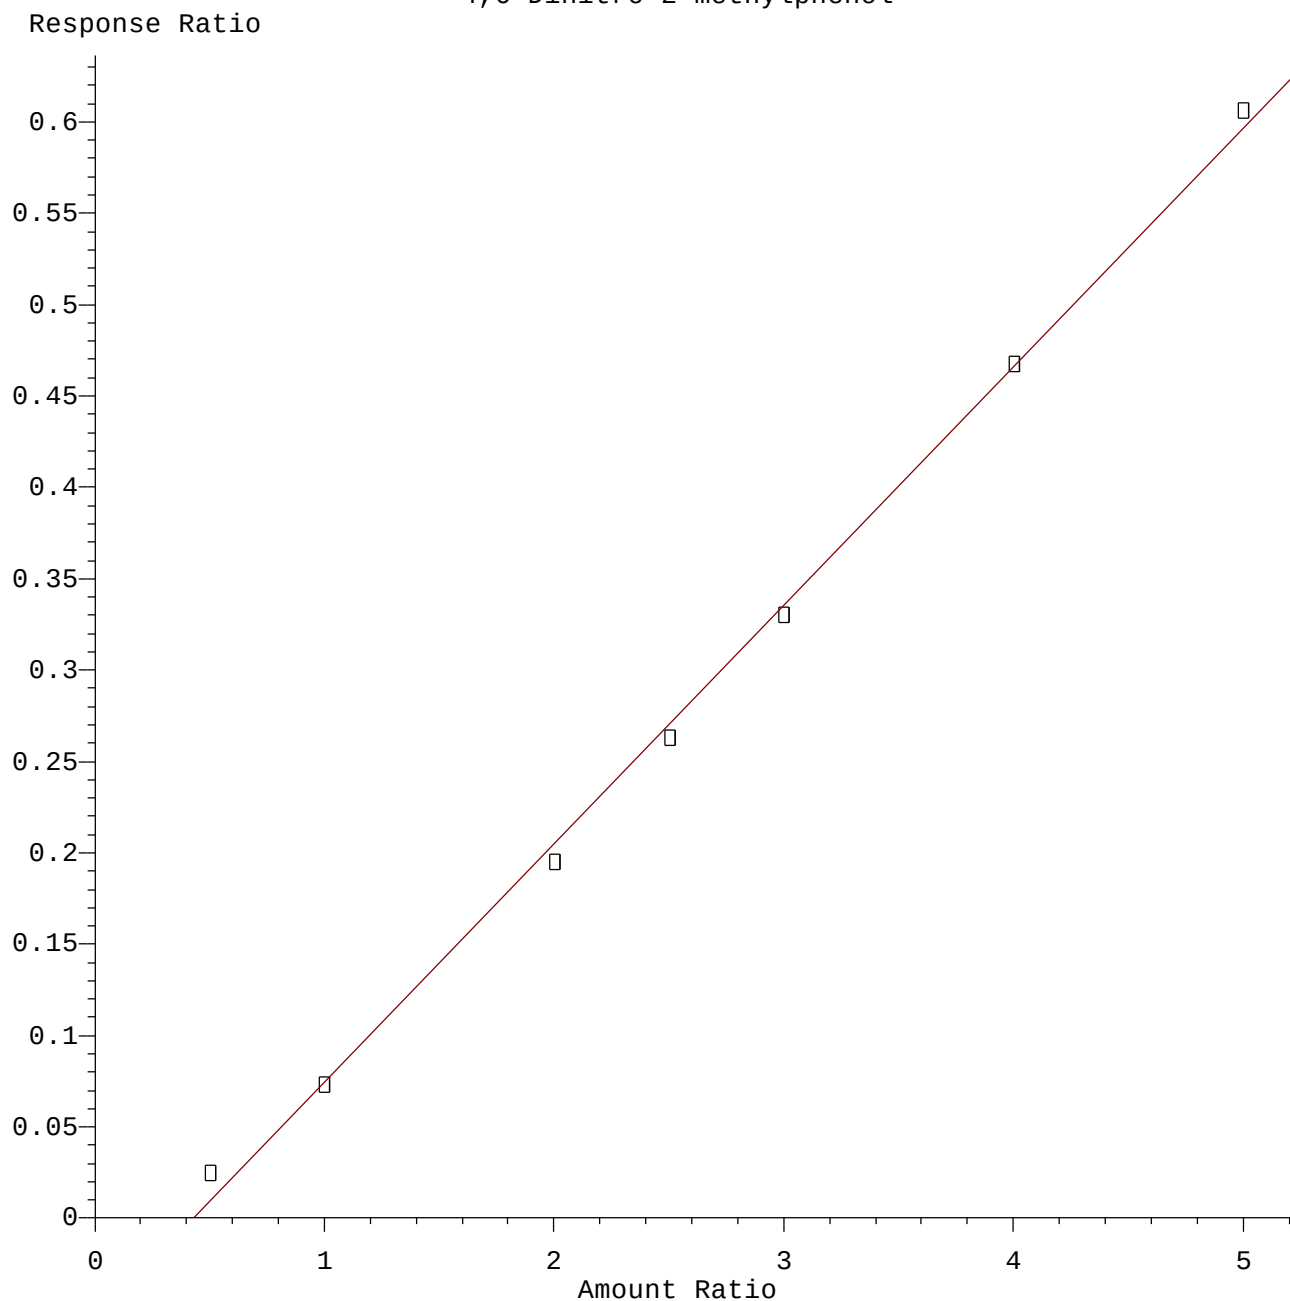


Resp Ratio = $1.31 \times 10^{-1} \times \text{Amt} - 5.61 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
Calibration Table Last Updated: Wed May 29 18:39:57 2019

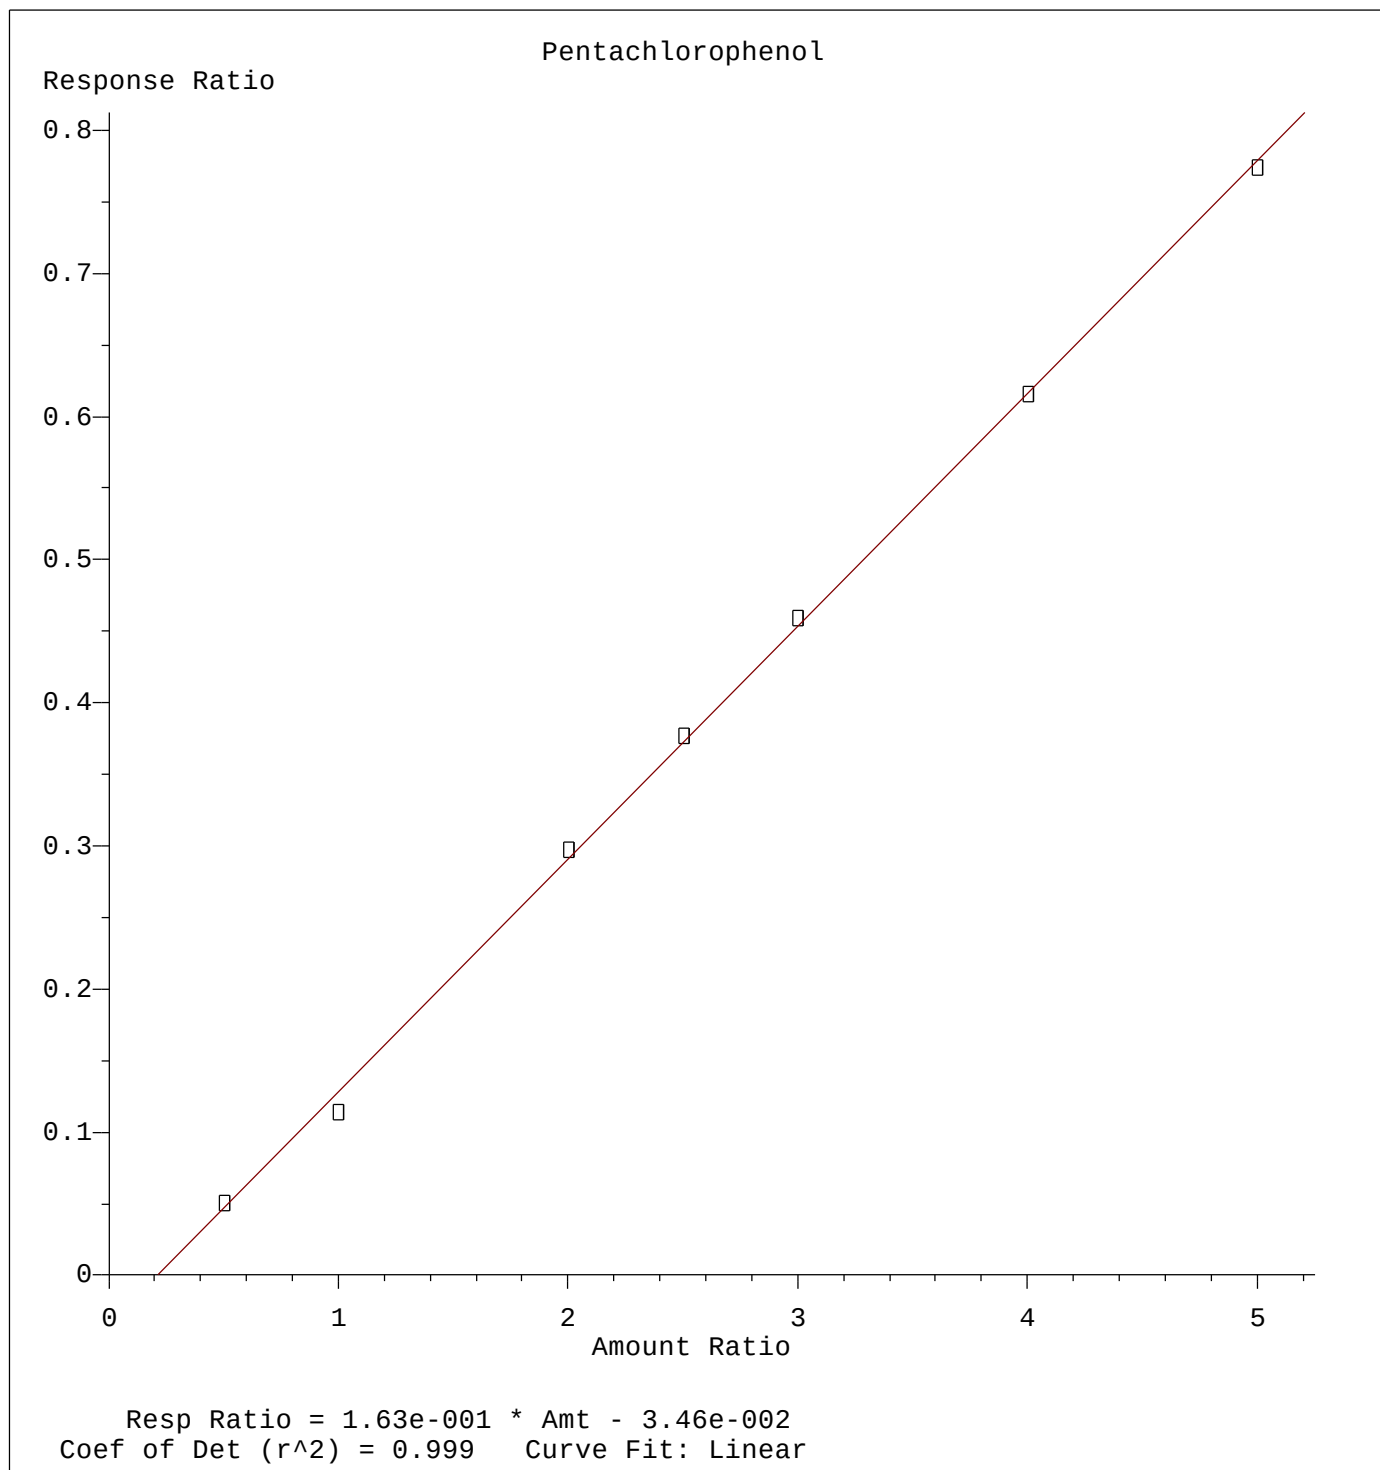

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
Calibration Table Last Updated: Wed May 29 18:39:57 2019

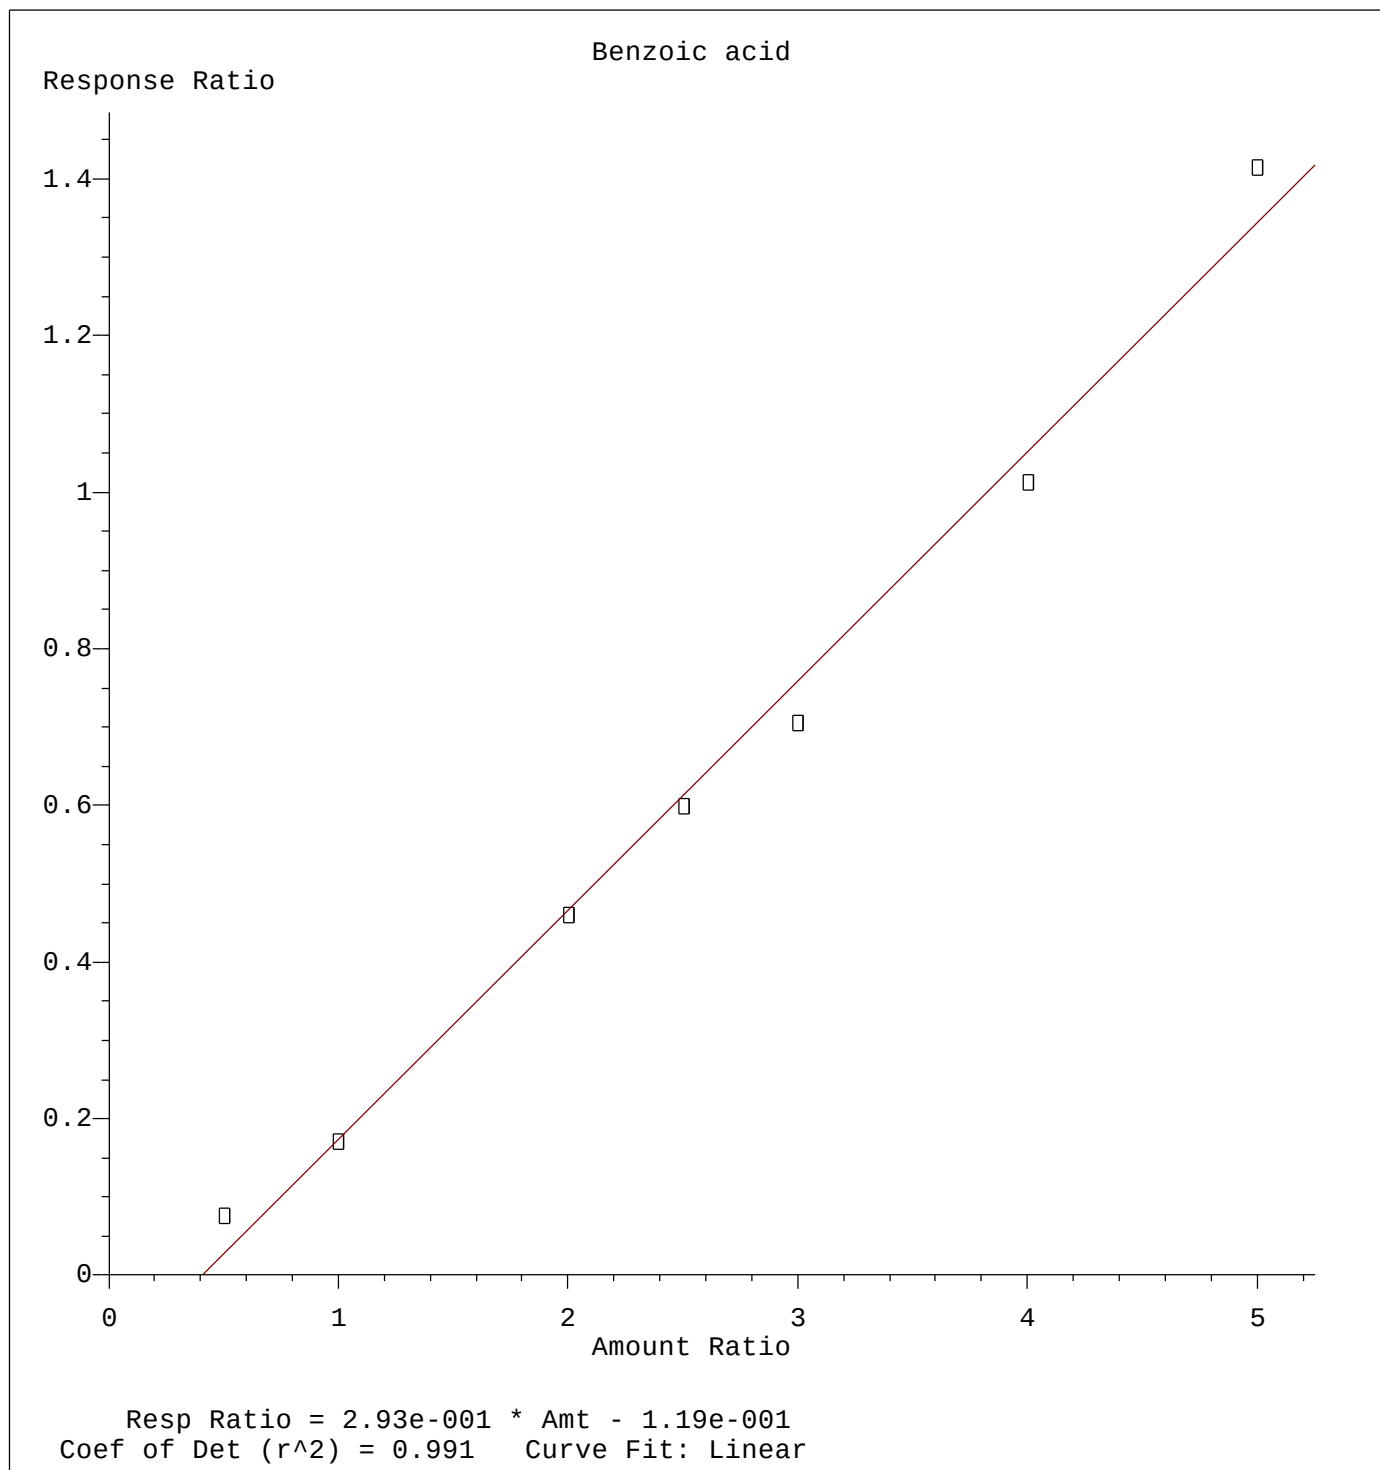

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
Calibration Table Last Updated: Wed May 29 18:39:57 2019