
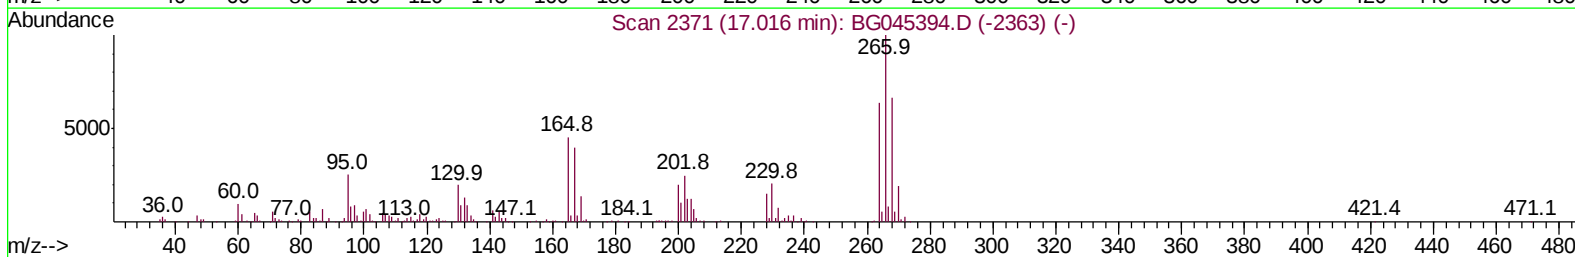
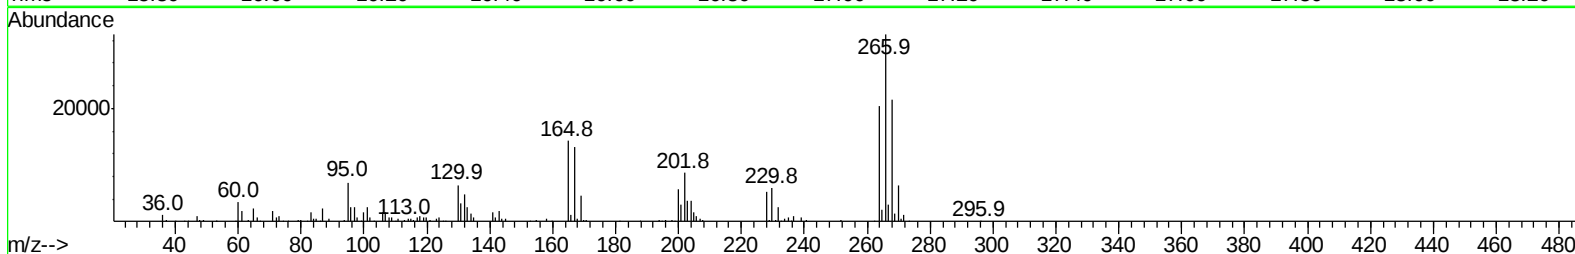


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG052920\
Data File : BG045534.D
Acq On : 29 May 2020 23:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 00:49:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 29 11:17:45 2020
Response via : Initial Calibration

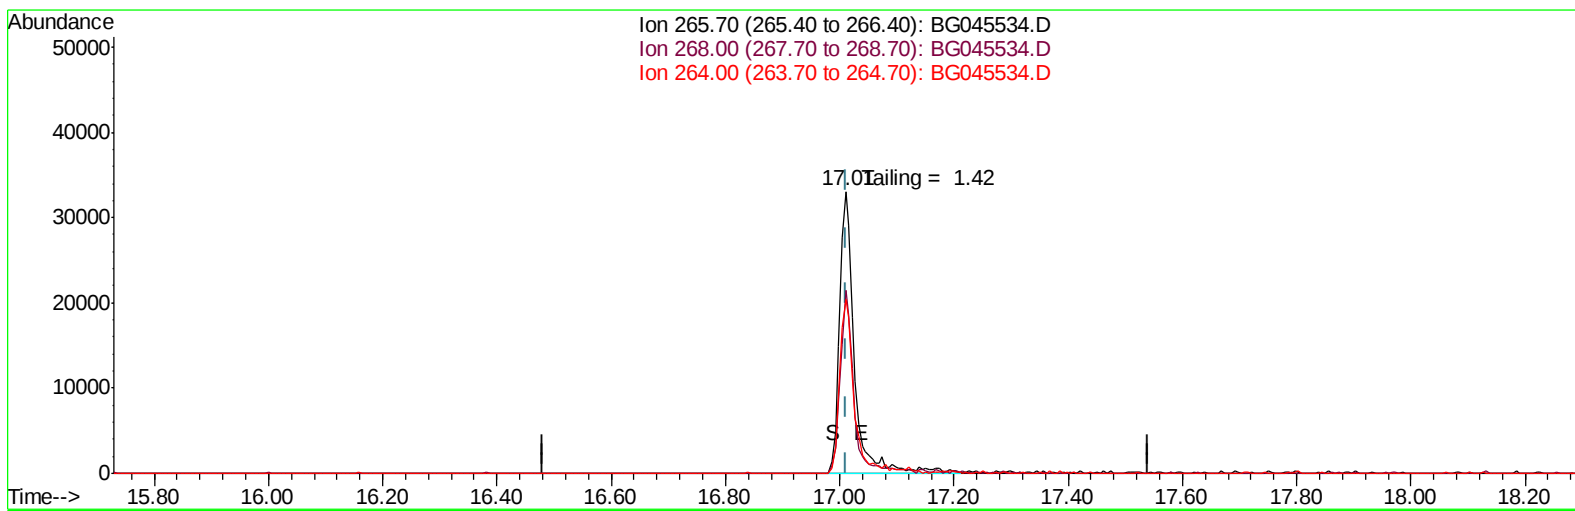

TIC: BG045534.D

(70) Pentachlorophenol (C)




17.010min (-0.001) 112298.98ng

response 56794

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	64.92
264.00	63.70	61.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG052920\
 Data File : BG045534.D
 Acq On : 29 May 2020 23:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 00:49:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 29 11:17:45 2020
 Response via : Initial Calibration

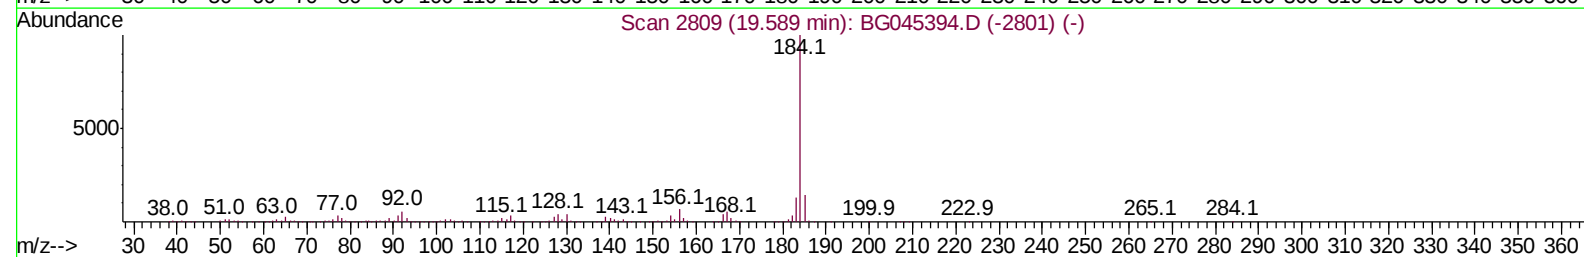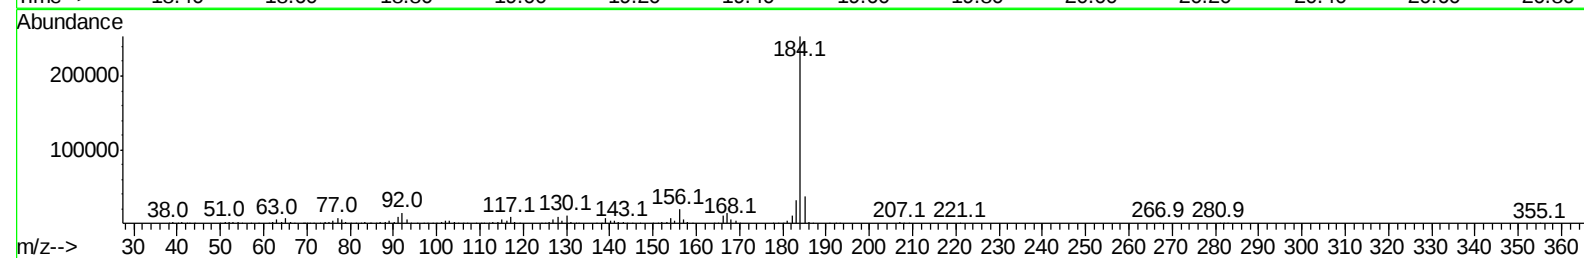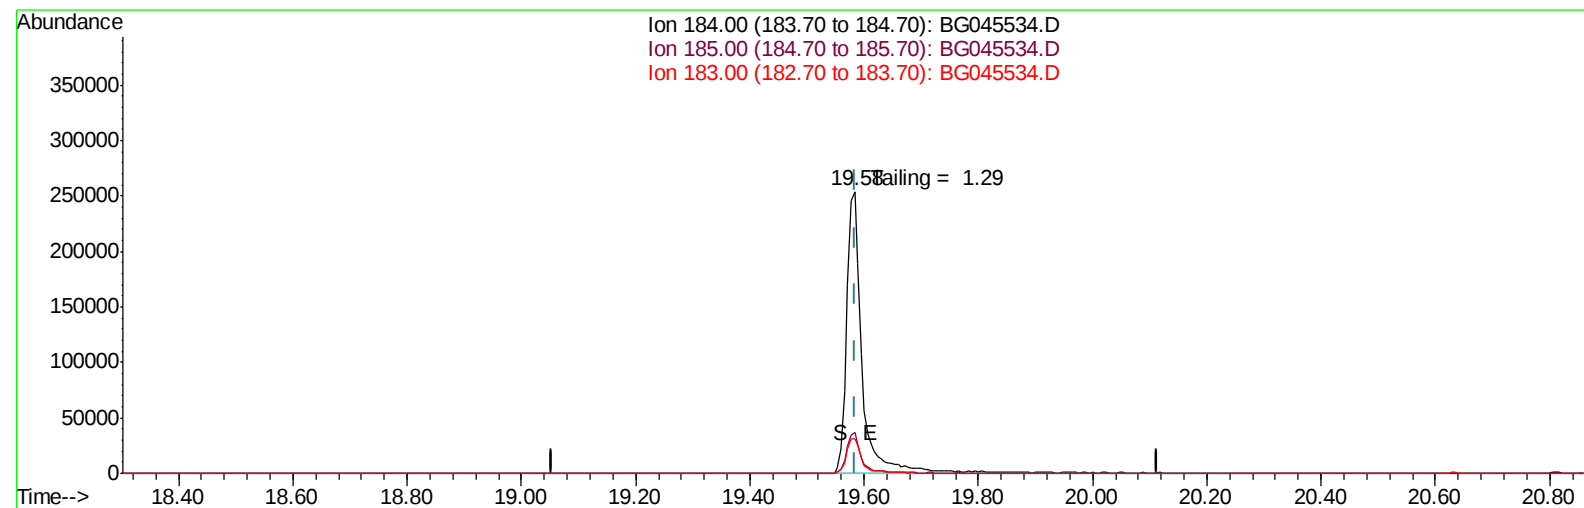

TIC: BG045534.D

(77) Benzidine

19.583min (-0.001) 312118.49ng

response 473364

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	14.53
183.00	12.80	12.33
0.00	0.00	0.00