
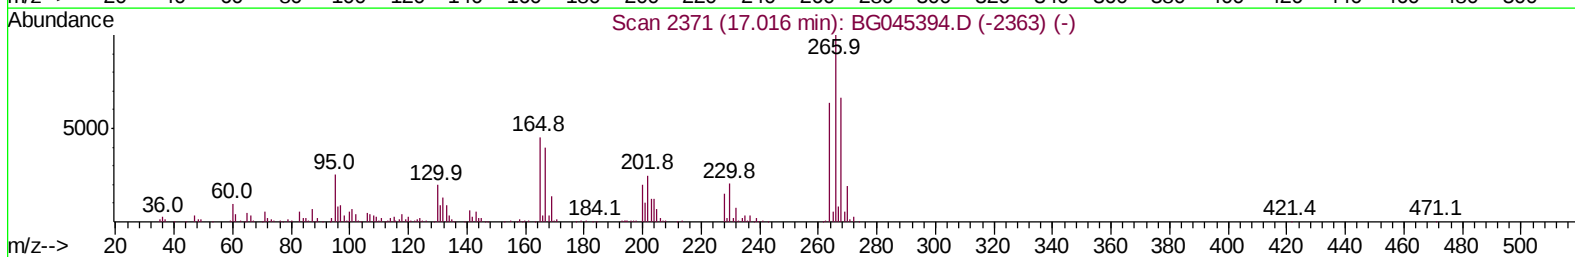
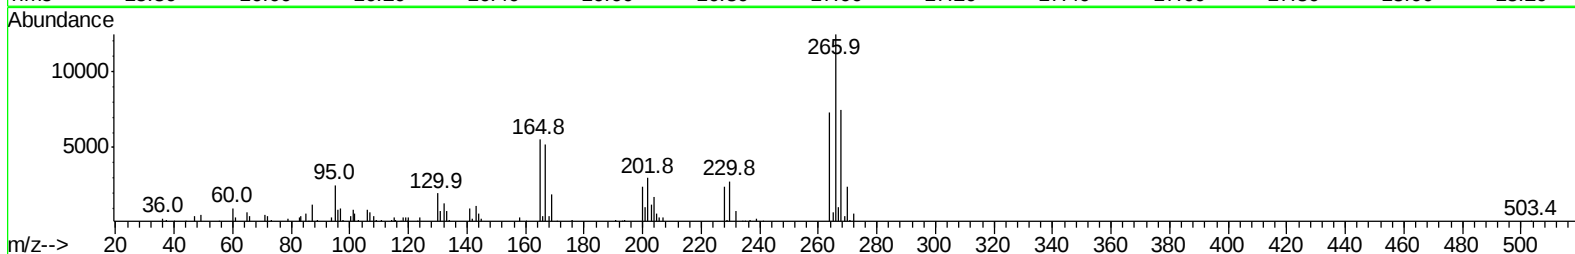


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG052920\  
 Data File : BG045549.D  
 Acq On : 30 May 2020 10:42  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 31 23:09:36 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri May 29 11:17:45 2020  
 Response via : Initial Calibration

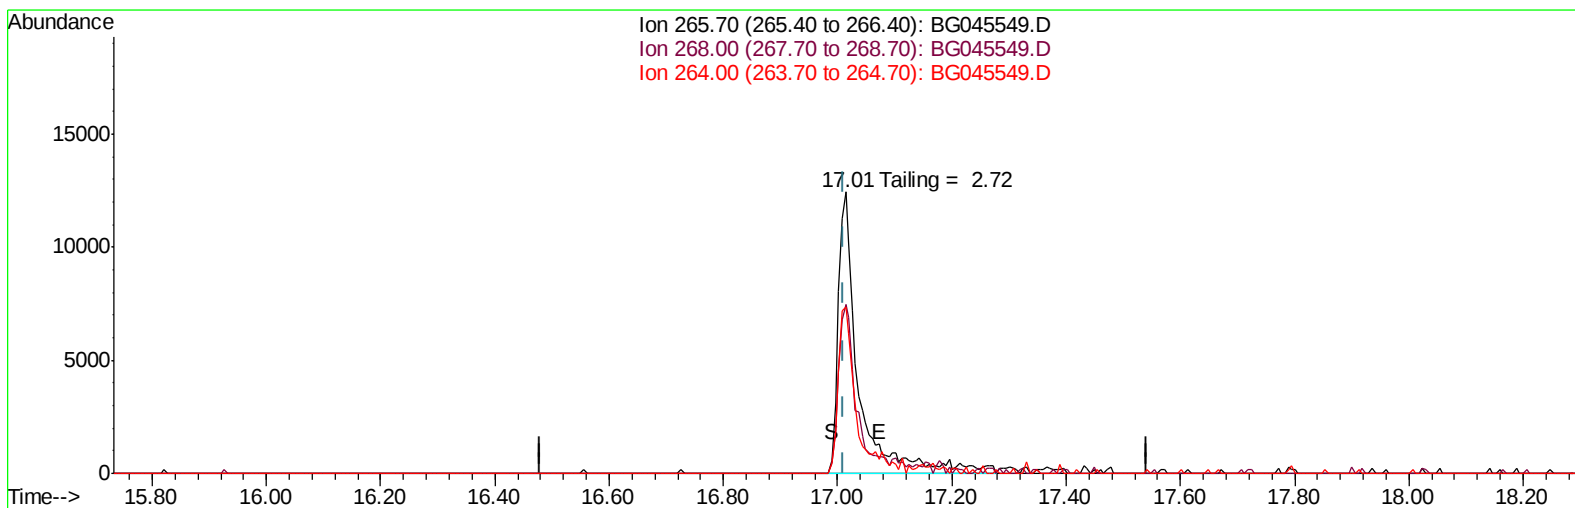

TIC: BG045549.D

(70) Pentachlorophenol (C)




17.013min (+0.002) 8120.49ng

response 26217

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 66.50 | 60.08 |
| 264.00 | 63.70 | 59.07 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG052920\  
 Data File : BG045549.D  
 Acq On : 30 May 2020 10:42  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 31 23:09:36 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri May 29 11:17:45 2020  
 Response via : Initial Calibration

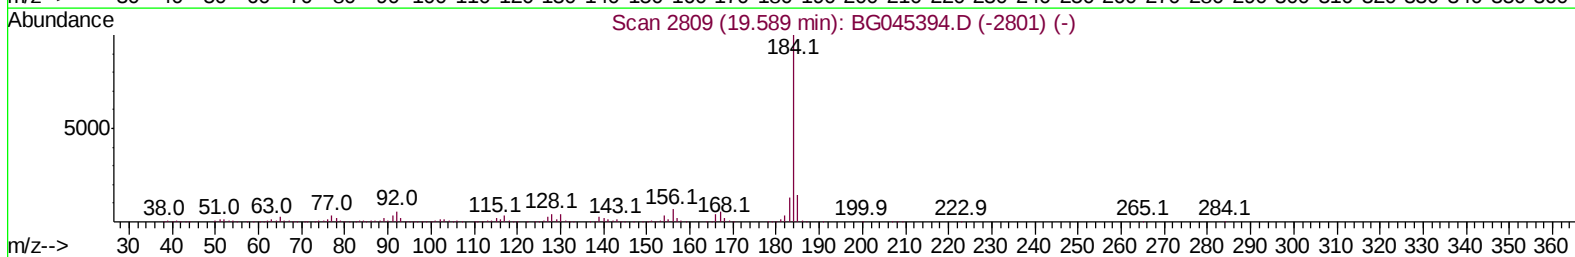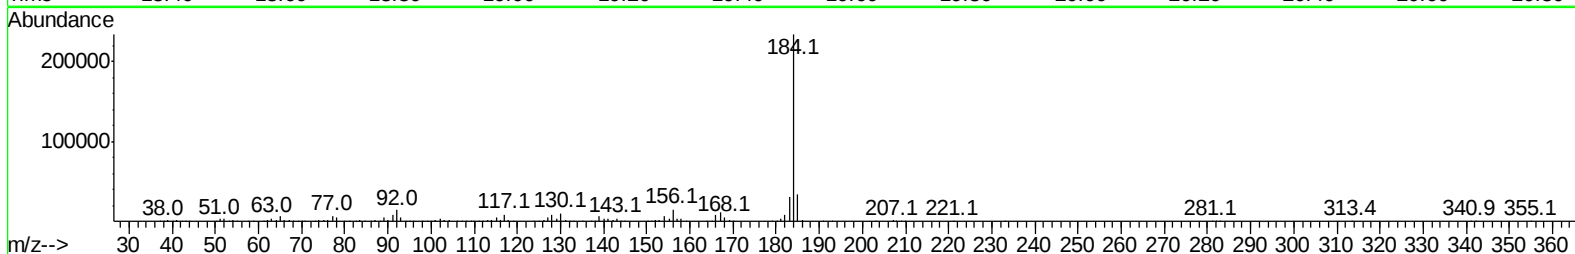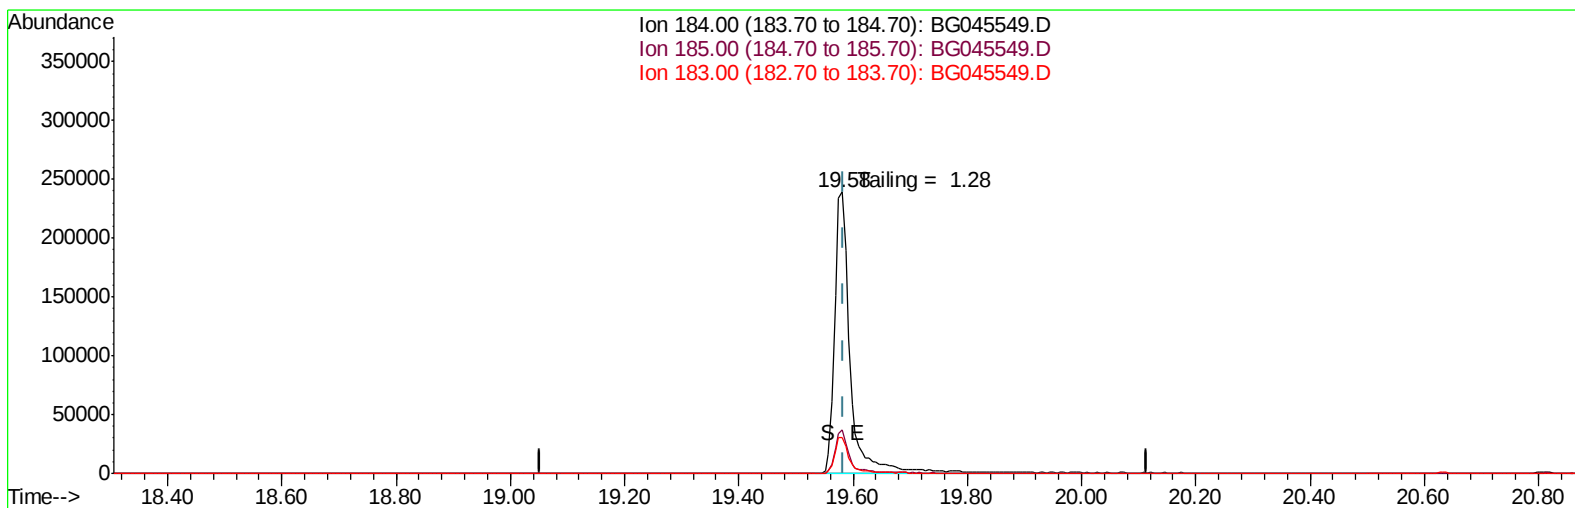

TIC: BG045549.D

(77) Benzidine

19.581min (-0.004) 234584.20ng

response 448012

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.60 | 15.31 |
| 183.00 | 12.80 | 12.73 |
| 0.00   | 0.00  | 0.00  |