


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052920\
 Data File : BG045534.D
 Acq On : 29 May 2020 23:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 01 15:07:00 2020

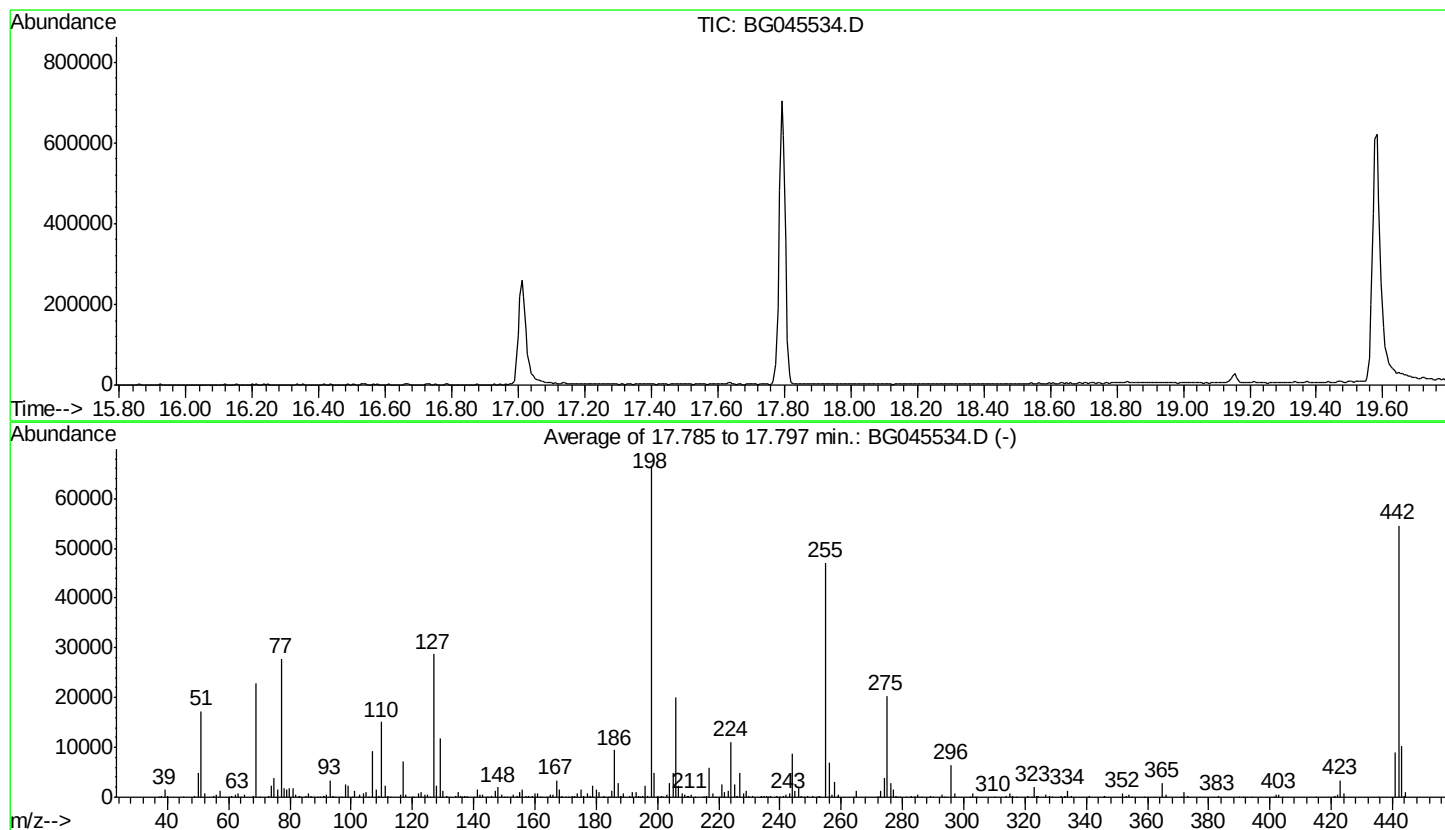

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.9	17269	PASS
68	69	0.00	2	0.7	164	PASS
69	198	0.00	100	34.2	22805	PASS
70	69	0.00	2	0.6	137	PASS
127	198	10	80	43.1	28736	PASS
197	198	0.00	2	0.3	232	PASS
198	198	100	100	100.0	66608	PASS
199	198	5	9	7.3	4853	PASS
275	198	10	60	30.6	20391	PASS
365	198	1	100	4.3	2858	PASS
441	198	0.01	100	13.6	9066	PASS
442	198	50	100	82.0	54618	PASS
443	442	15	24	18.8	10291	PASS