


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052920\
 Data File : BG045549.D
 Acq On : 30 May 2020 10:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 01 15:07:00 2020

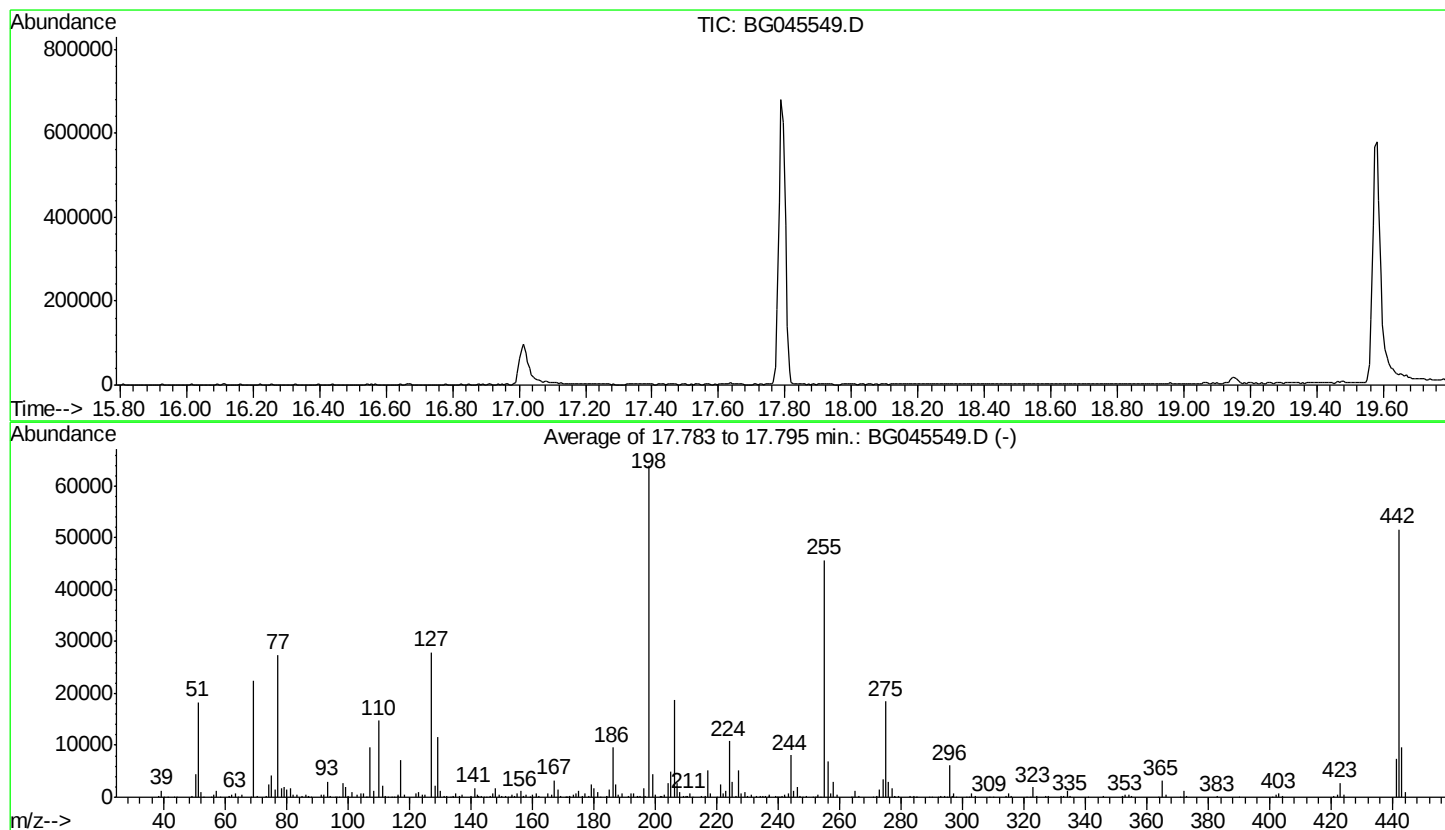

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	18360	PASS
68	69	0.00	2	0.5	116	PASS
69	198	0.00	100	35.3	22530	PASS
70	69	0.00	2	0.8	175	PASS
127	198	10	80	43.7	27933	PASS
197	198	0.00	2	0.4	224	PASS
198	198	100	100	100.0	63912	PASS
199	198	5	9	6.9	4380	PASS
275	198	10	60	28.8	18394	PASS
365	198	1	100	5.0	3206	PASS
441	198	0.01	100	11.6	7392	PASS
442	198	50	100	80.7	51589	PASS
443	442	15	24	18.9	9746	PASS