

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053024\
 Data File : BG061364.D
 Acq On : 30 May 2024 17:52
 Operator : MA/JU
 Sample : P2635-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH5S2

Quant Time: May 30 22:56:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 30 22:54:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.870	152	25039	20.000	ng/ul	0.00
20) Naphthalene-d8	10.667	136	86952	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.509	164	69662	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.253	188	177477	20.000	ng/ul	0.00
79) Chrysene-d12	21.507	240	184152	20.000	ng/ul	0.00
88) Perylene-d12	24.592	264	206459	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	2802	6.263	ng/uL	0.00
4) Pyridine-d5	3.745	84	18527	11.639	ng/ul	0.00
7) Phenol-d5	7.053	99	14953	7.272	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.200	67	47740	36.938	ng/ul	0.00
11) 2-Chlorophenol-d4	7.412	132	41993	27.595	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	26265	14.980	ng/ul	0.00
21) Nitrobenzene-d5	9.027	128	26297	39.280	ng/ul	0.00
24) 2-Nitrophenol-d4	9.750	143	17488	22.320	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.302	165	49271	32.257	ng/ul	0.00
31) 4-Chloroaniline-d4	10.802	131	67449	33.752	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166	217300	40.220	ng/ul	0.00
49) Acenaphthylene-d8	14.198	160	226415	40.309	ng/ul	0.00
54) 4-Nitrophenol-d4	14.768	143	351	0.525	ng/ul	0.03
60) Fluorene-d10	15.502	176	188296	40.367	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	
73) Anthracene-d10	17.359	188	348093	44.488	ng/ul	0.00
81) Pyrene-d10	19.650	212	415054	43.896	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.380	264	440750	44.405	ng/ul	0.00
Target Compounds						
59) Diethylphthalate	15.326	149	9512	1.711	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053024\
Data File : BG061364.D
Acq On : 30 May 2024 17:52
Operator : MA/JU
Sample : P2635-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH5S2


Quant Time: May 30 22:56:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 30 22:54:48 2024
Response via : Initial Calibration

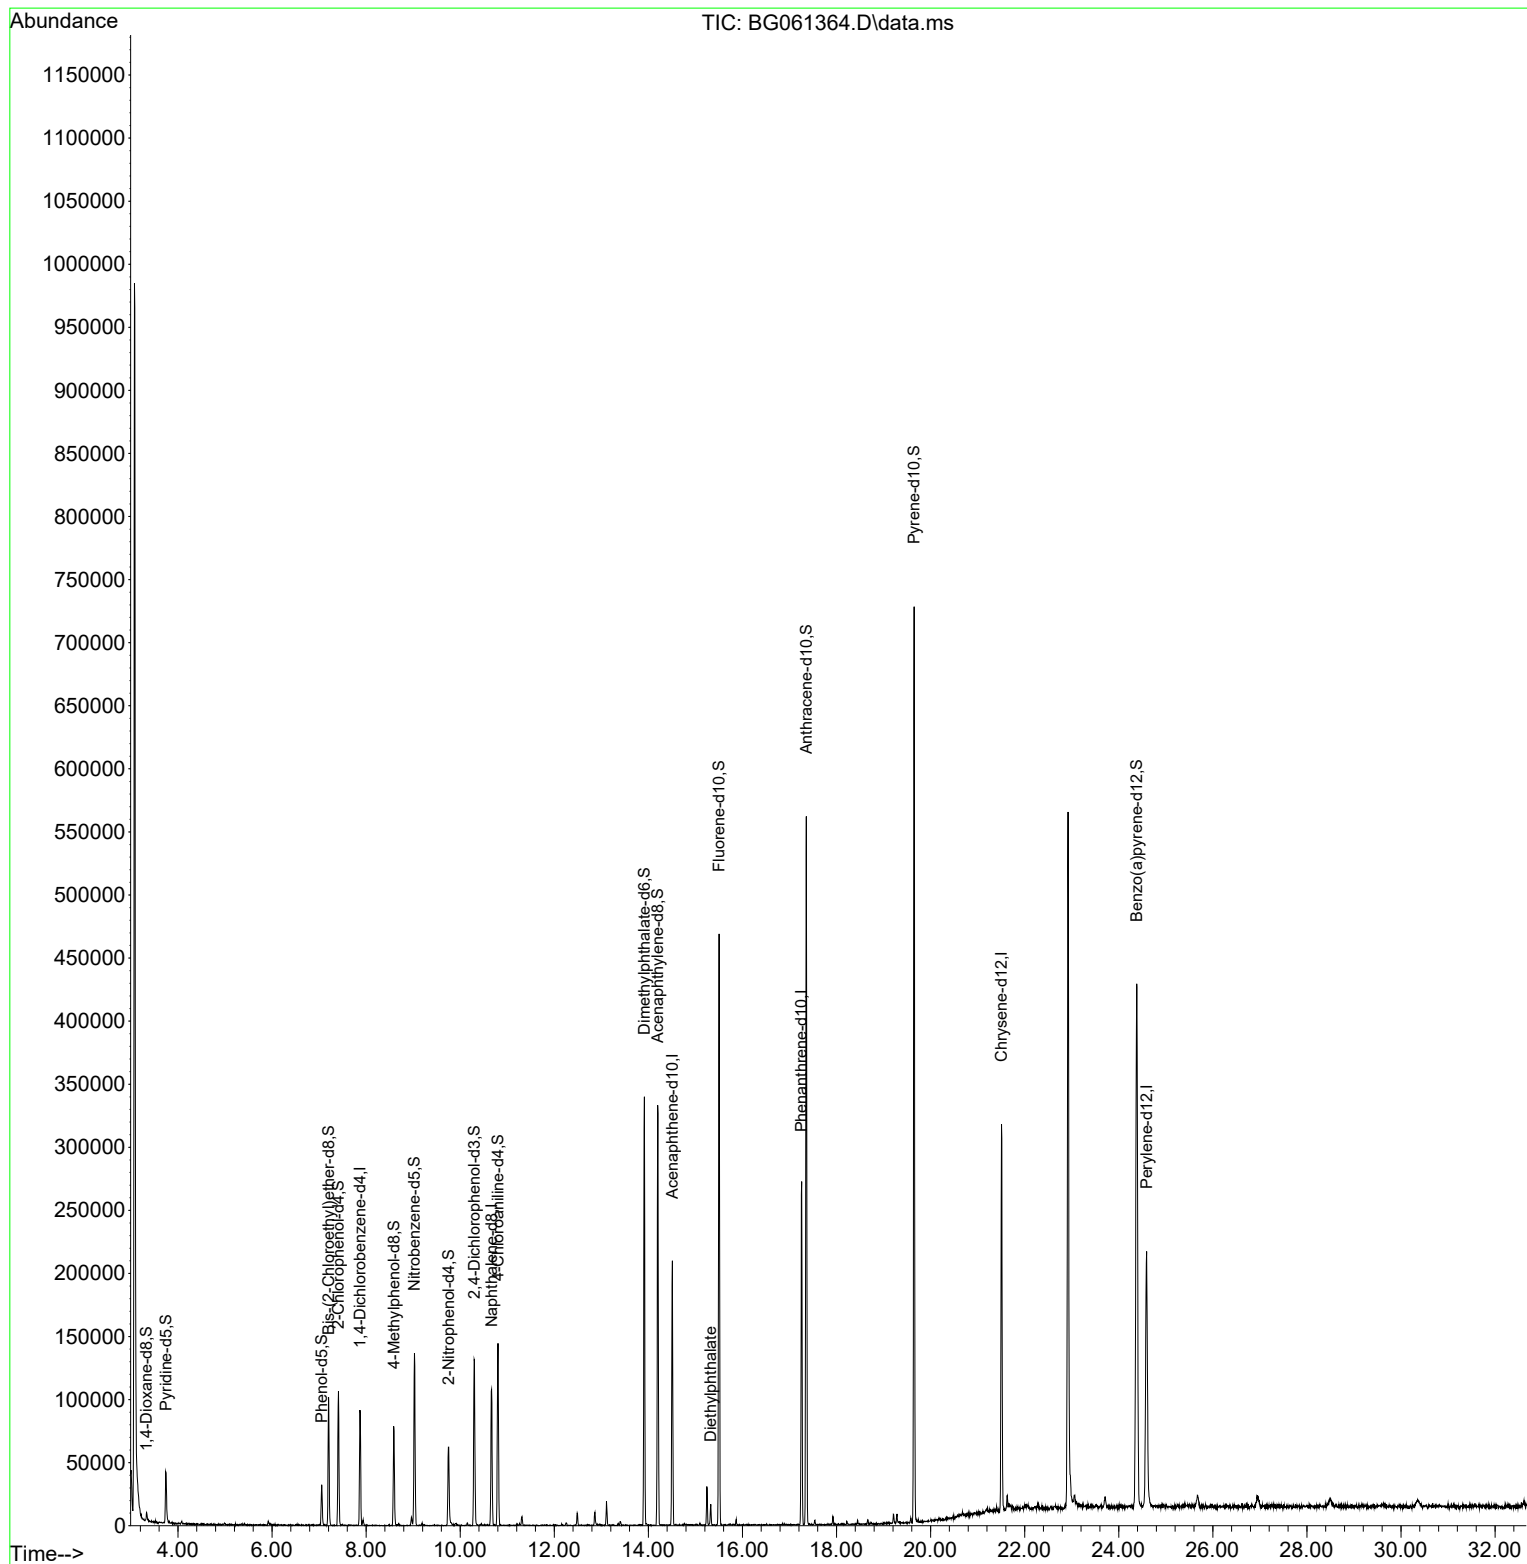

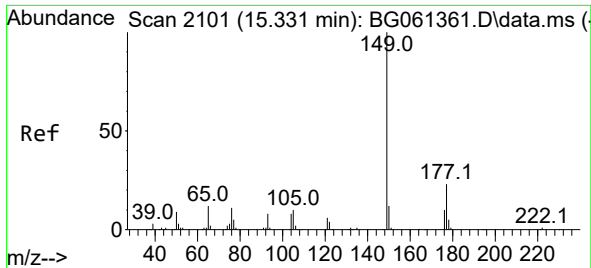

#59
 Diethylphthalate
 Concen: 1.711 ng/ul
 RT: 15.326 min Scan# 21
 Delta R.T. -0.005 min
 Lab File: BG061364.D
 Acq: 30 May 2024 17:52

Instrument :
 BNA_G
 ClientSampleId :
 BH5S2

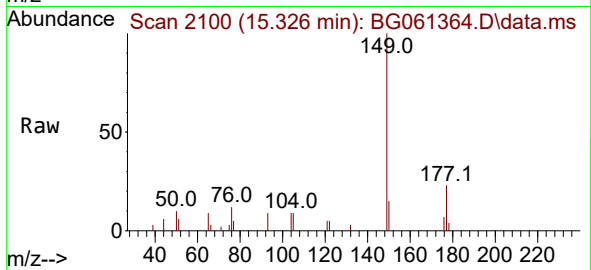

Tgt Ion:	149	Resp:	9512
Ion Ratio	Lower	Upper	
149	100		
177	23.2	19.1	28.7
150	15.2	11.0	16.4

